



SPC BENCHMARK 1™
FULL DISCLOSURE REPORT

HUAWEI TECHNOLOGIES Co., LTD.
HUAWEI OCEANSTOR™ 5600 V3

SPC-1 V1.14

Submitted for Review: April 26, 2016
Submission Identifier: A00175

First Edition – April 2016

THE INFORMATION CONTAINED IN THIS DOCUMENT IS DISTRIBUTED ON AN AS IS BASIS WITHOUT ANY WARRANTY EITHER EXPRESS OR IMPLIED. The use of this information or the implementation of any of these techniques is the customer's responsibility and depends on the customer's ability to evaluate and integrate them into the customer's operational environment. While each item has been reviewed by Huawei Technologies Co., Ltd. for accuracy in a specific situation, there is no guarantee that the same or similar results will be obtained elsewhere. Customers attempting to adapt these techniques to their own environment do so at their own risk.

This publication was produced in the United States. Huawei Technologies Co., Ltd. may not offer the products, services, or features discussed in this document in other countries, and the information is subject to change with notice. Consult your local Huawei Technologies Co., Ltd. representative for information on products and services available in your area.

© Copyright Huawei Technologies Co., Ltd. 2016. All rights reserved.

Permission is hereby granted to reproduce this document in whole or in part, provided the copyright notice as printed above is set forth in full text on the title page of each item reproduced.

Trademarks

SPC Benchmark-1, SPC-1, SPC-1 IOPS, SPC-1 LRT and SPC-1 Price-Performance are trademarks of the Storage Performance Council. Huawei, the Huawei logo and OceanStor are trademarks or registered trademarks of Huawei Technologies Co., Ltd. in the United States and other countries. All other brands, trademarks, and product names are the property of their respective owners.

Table of Contents

Audit Certification.....	vii
Audit Certification (<i>cont.</i>)	viii
Letter of Good Faith	ix
Executive Summary.....	10
Test Sponsor and Contact Information.....	10
Revision Information and Key Dates	10
Tested Storage Product (TSP) Description.....	11
Summary of Results	12
Storage Capacities, Relationships, and Utilization	13
Response Time – Throughput Curve	16
Response Time – Throughput Data.....	16
Priced Storage Configuration Pricing	17
Differences between the Tested Storage Configuration (TSC) and Priced Storage Configuration.....	18
Priced Storage Configuration Diagram.....	19
Priced Storage Configuration Components.....	20
Configuration Information	21
Benchmark Configuration (BC)/Tested Storage Configuration (TSC) Diagram.....	21
Storage Network Configuration	21
Host System(s) and Tested Storage Configuration (TSC) Table of Components	21
Benchmark Configuration/Tested Storage Configuration Diagram.....	22
Host System and Tested Storage Configuration Components	23
Benchmark Configuration/Tested Storage Configuration Connections.....	24
Host System, FC HBA, Engine, Controller, FC Host Port Module/Ports	24
Host System to Controller Host Port FC Connections	24
Engine, Controller, Eth/FCoE Module/Active Port Relationships	25
Controller-to-Controller Eth/FCoE Connections	26
Controller to Controller Eth/FCoE Connections (<i>continued</i>)	27
Engine, Controller and SAS Module/Active Port Relationships.....	28
Controller/Disk Enclosure SAS Connections	29
Customer Tunable Parameters and Options	30
Tested Storage Configuration (TSC) Description	30
SPC-1 Workload Generator Storage Configuration	30
ASU Pre-Fill.....	31
SPC-1 Data Repository.....	32
Storage Capacities and Relationships	32

SPC-1 Storage Capacities	32
SPC-1 Storage Hierarchy Ratios	33
SPC-1 Storage Capacity Charts	33
Storage Capacity Utilization	35
Logical Volume Capacity and ASU Mapping.....	36
SPC-1 Benchmark Execution Results.....	37
SPC-1 Tests, Test Phases, and Test Runs.....	37
“Ramp-Up” Test Runs.....	38
Primary Metrics Test – Sustainability Test Phase	38
SPC-1 Workload Generator Input Parameters	39
Sustainability Test Results File	39
Sustainability – Data Rate Distribution Data (MB/second)	39
Sustainability – Data Rate Distribution Graph	39
Sustainability – I/O Request Throughput Distribution Data	40
Sustainability – I/O Request Throughput Distribution Graph	40
Sustainability – Average Response Time (ms) Distribution Data	41
Sustainability – Average Response Time (ms) Distribution Graph	41
Sustainability – Response Time Frequency Distribution Data	42
Sustainability – Response Time Frequency Distribution Graph	42
Sustainability – Measured Intensity Multiplier and Coefficient of Variation.....	43
Primary Metrics Test – IOPS Test Phase.....	44
SPC-1 Workload Generator Input Parameters	44
IOPS Test Results File.....	44
IOPS Test Run – I/O Request Throughput Distribution Data	45
IOPS Test Run – I/O Request Throughput Distribution Graph.....	45
IOPS Test Run – Average Response Time (ms) Distribution Data	46
IOPS Test Run – Average Response Time (ms) Distribution Graph	46
IOPS Test Run – Response Time Frequency Distribution Data	47
IOPS Test Run – Response Time Frequency Distribution Graph.....	47
IOPS Test Run – I/O Request Information.....	48
IOPS Test Run – Measured Intensity Multiplier and Coefficient of Variation	48
Primary Metrics Test – Response Time Ramp Test Phase	49
SPC-1 Workload Generator Input Parameters	49
Response Time Ramp Test Results File.....	49
Response Time Ramp Distribution (IOPS) Data.....	50
Response Time Ramp Distribution (IOPS) Data (<i>continued</i>)	51
Response Time Ramp Distribution (IOPS) Graph	51
SPC-1 LRT™ Average Response Time (ms) Distribution Data.....	52
SPC-1 LRT™ Average Response Time (ms) Distribution Graph	52

SPC-1 LRT™ (10%) – Measured Intensity Multiplier and Coefficient of Variation	53
Repeatability Test	54
SPC-1 Workload Generator Input Parameters	54
Repeatability Test Results File	55
Repeatability 1 LRT – I/O Request Throughput Distribution Data.....	56
Repeatability 1 LRT – I/O Request Throughput Distribution Graph	56
Repeatability 1 LRT –Average Response Time (ms) Distribution Data	57
Repeatability 1 LRT –Average Response Time (ms) Distribution Graph.....	57
Repeatability 1 IOPS – I/O Request Throughput Distribution Data	58
Repeatability 1 IOPS – I/O Request Throughput Distribution Graph.....	58
Repeatability 1 IOPS –Average Response Time (ms) Distribution Data.....	59
Repeatability 1 IOPS –Average Response Time (ms) Distribution Graph	59
Repeatability 2 LRT – I/O Request Throughput Distribution Data.....	60
Repeatability 2 LRT – I/O Request Throughput Distribution Graph	60
Repeatability 2 LRT –Average Response Time (ms) Distribution Data	61
Repeatability 2 LRT –Average Response Time (ms) Distribution Graph.....	61
Repeatability 2 IOPS – I/O Request Throughput Distribution Data	62
Repeatability 2 IOPS – I/O Request Throughput Distribution Graph.....	62
Repeatability 2 IOPS –Average Response Time (ms) Distribution Data	63
Repeatability 2 IOPS –Average Response Time (ms) Distribution Graph	63
Repeatability 1 (LRT) Measured Intensity Multiplier and Coefficient of Variation	64
Repeatability 1 (IOPS) Measured Intensity Multiplier and Coefficient of Variation	64
Repeatability 2 (LRT) Measured Intensity Multiplier and Coefficient of Variation	64
Repeatability 2 (IOPS) Measured Intensity Multiplier and Coefficient of Variation	65
Data Persistence Test.....	66
SPC-1 Workload Generator Input Parameters	66
Data Persistence Test Results File	66
Data Persistence Test Results.....	67
Priced Storage Configuration Availability Date.....	68
Pricing Information.....	68
Tested Storage Configuration (TSC) and Priced Storage Configuration Differences.....	68
Anomalies or Irregularities	68
Appendix A: SPC-1 Glossary	69
“Decimal” (<i>powers of ten</i>) Measurement Units	69
“Binary” (<i>powers of two</i>) Measurement Units.....	69
SPC-1 Data Repository Definitions.....	69
SPC-1 Data Protection Levels	70

SPC-1 Test Execution Definitions	70
I/O Completion Types	72
SPC-1 Test Run Components	72
Appendix B: Customer Tunable Parameters and Options.....	73
Red Hat Enterprise Linux 7.0 (64-bit)	73
Appendix C: Tested Storage Configuration (TSC) Creation	74
Step 1: Create Mapping View, LUN Group, Host Group and Host.....	74
Step 2: Create Disk Domains, Storage Pools, LUNs	75
Step 3: Create Volumes on the Master Host System	75
Step 4: Change the Scheduler on each Host System.....	76
Referenced Scripts.....	76
mklun.sh	76
mkvolume.sh	78
scheduler.sh.....	79
Appendix D: SPC-1 Workload Generator Storage Commands and Parameters	80
ASU Pre-Fill.....	80
Primary Metrics and Repeatability Tests	81
SPC-1 Persistence.....	82
Appendix E: SPC-1 Workload Generator Input Parameters	83
run.sh	83
Appendix F: Third-Party Quotation.....	86
Priced Storage Configuration	86
Priced Storage Configuration (<i>continued</i>).....	87

AUDIT CERTIFICATION



Gradient
SYSTEMS

Xu Zhong
 Huawei Technologies Co., Ltd.
 Huawei Chengdu Base
 No. 1899, Xiyuan Avenue
 Chengdu, 611731 P.R. China

April 25, 2016

The SPC Benchmark 1™ Reported Data listed below for the Huawei OceanStor™ 5600 V3 was produced in compliance with the SPC Benchmark 1™ v1.14 Remote Audit requirements.

SPC Benchmark 1™ v1.14 Reported Data	
Tested Storage Product (TSP) Name:	
Metric	Reported Result
SPC-1 IOPS™	401,005.47
SPC-1 Price-Performance	\$0.35/SPC-1 IOPS™
Total ASU Capacity	8,504.035 GB
Data Protection Level	Protected 2 (<i>Mirroring</i>)
Total Price (including three-year maintenance)	\$81,900.78
Currency Used	U.S. Dollars
Target Country for availability, sales and support	USA

The following SPC Benchmark 1™ Remote Audit requirements were reviewed and found compliant with 1.14 of the SPC Benchmark 1™ specification:

- A Letter of Good Faith, signed by a senior executive.
- The following Data Repository storage items were verified by information supplied by Huawei Technologies Co., Ltd:
 - ✓ Physical Storage Capacity and requirements.
 - ✓ Configured Storage Capacity and requirements.
 - ✓ Addressable Storage Capacity and requirements.
 - ✓ Capacity of each Logical Volume and requirements.
 - ✓ Capacity of each Application Storage Unit (ASU) and requirements.
- The total Application Storage Unit (ASU) Capacity was filled with random data, using an auditor approved tool, prior to execution of the SPC-1 Tests.

Gradient Systems, Inc.
 643 Bair Island Road, Suite 103
 Redwood City, CA 94062
AuditService@storageperformance.org
 650.556.9384

AUDIT CERTIFICATION (CONT.)

Huawei OceanStor™ 5600 V3
SPC-1 Audit Certification


Page 2

- An appropriate diagram of the Benchmark Configuration (BC)/Tested Storage Configuration (TSC).
- Listings and commands to configure the Benchmark Configuration/Tested Storage Configuration, including customer tunable parameters that were changed from default values.
- SPC-1 Workload Generator commands and parameters used for the audited SPC Test Runs.
- The following Host System requirements were verified by information supplied by Huawei Technologies Co., Ltd.:
 - ✓ The type of Host Systems including the number of processors and main memory.
 - ✓ The presence and version number of the SPC-1 Workload Generator on each Host System.
 - ✓ The TSC boundary within each Host System.
- The execution of each Test, Test Phase, and Test Run was found compliant with all of the requirements and constraints of Clauses 4, 5, and 11 of the SPC-1 Benchmark Specification.
- The Test Results Files and resultant Summary Results Files received from Huawei Technologies Co., Ltd. for each of following were authentic, accurate, and compliant with all of the requirements and constraints of Clauses 4 and 5 of the SPC-1 Benchmark Specification:
 - ✓ Data Persistence Test
 - ✓ Sustainability Test Phase
 - ✓ IOPS Test Phase
 - ✓ Response Time Ramp Test Phase
 - ✓ Repeatability Test
- There were no differences between the Tested Storage Configuration (TSC) and Priced Storage Configuration.
- The submitted pricing information met all of the requirements and constraints of Clause 8 of the SPC-1 Benchmark Specification.
- The Full Disclosure Report (FDR) met all of the requirements in Clause 9 of the SPC-1 Benchmark Specification.
- This successfully audited SPC measurement is not subject to an SPC Confidential Review.

Audit Notes:

There were no audit notes or exceptions.

Respectfully,



Walter E. Baker
SPC Auditor

Gradient Systems, Inc.
643 Bair Island Road, Suite 103
Redwood City, CA 94062
AuditService@storageperformance.org
650.556.9384

LETTER OF GOOD FAITH



©Huawei Technologies Co., Ltd.
 Huawei Industrial Base, Bantian, Longgang
 Shenzhen city
 Guangdong province
 China
 Tel: 0086-755-28780808
<http://www.huawei.com/en/>

Date: April 7, 2016

From: Huawei Technologies Co., Ltd.

To: Walter E. Baker, SPC Auditor
 Gradient Systems, Inc.
 643 Bair Island Road. Suite 103
 Redwood City, CA 94063

Subject: SPC-1 Letter of Good Faith for the Huawei OceanStor 5600 V3

Huawei Technologies Co., Ltd. is the SPC-1 Test Sponsor for the above listed product. To the best of our knowledge and belief, the required SPC-1 benchmark results and materials we have submitted for that product are complete, accurate, and in full compliance with V1.14 of the SPC-1 benchmark specification.

In addition, we have reported any items in the Benchmark Configuration and execution of the benchmark that affected the reported results even if the items are not explicitly required to be disclosed by the SPC-1 benchmark specification.

Signed:

Fan Ruiqi
 President of Storage Product Line

Date:

EXECUTIVE SUMMARY

Test Sponsor and Contact Information

Test Sponsor and Contact Information	
Test Sponsor Primary Contact	Huawei Technologies Co., Ltd. – http://www.huawei.com/en/ Xu Zhong – xuzhong@huawei.com Huawei Chengdu Base No. 1899, Xiyuan Avenue Chengdu, 611731 P.R. China Phone: 86 28 65281927 FAX: 86 28 62282516
Test Sponsor Alternate Contact	Huawei Technologies Co., Ltd. – http://www.huawei.com/en/ Li Huan – tomas.l@huawei.com Huawei Chengdu Base No. 1899, Xiyuan Avenue Chengdu, 611731 P.R. China Phone: 86 28 65281927 FAX: 86 28 62282516
Auditor	Storage Performance Council – http://www.storageperformance.org Walter E. Baker – AuditService@StoragePerformance.org 643 Bair Island Road, Suite 103 Redwood City, CA 94063 Phone: (650) 556-9384 FAX: (650) 556-9385

Revision Information and Key Dates

Revision Information and Key Dates	
SPC-1 Specification revision number	V1.14
SPC-1 Workload Generator revision number	V2.3.0
Date Results were first used publicly	April 26, 2016
Date the FDR was submitted to the SPC	April 26, 2016
Date the Priced Storage Configuration is available for shipment to customers	currently available
Date the TSC completed audit certification	April 25, 2016

Tested Storage Product (TSP) Description

The Huawei OceanStor™ 5600 V3 offers a cloud architecture-oriented operating system, high-performance hardware platform, and a complete suite of smart management software. The product is scalable to eight controllers, 512 GB cache, a maximum of 1,000 storage devices, with a variety of interfaces, including 16 Gbit/s FC, 56 Gbit/s InfiniBand, PCIe 3.0, 12 Gbit/s SAS, and smart I/O cards.

The Huawei OceanStor™ 5600 V3 is a perfect storage system for large OLTP/OLAP databases, file sharing, and cloud computing in the government, finance, telecom, energy, and media industries.

OceanStor OS, the Huawei OceanStor storage operating system, enables Huawei storage products evolve to the future cloud architecture and deliver the core business platform. It supports all OceanStor Storage arrays, specifically, for managing the underlying infrastructure, the physical space and logical space. OceanStor OS delivers intelligent and convergent services and multiple SLAs to the application scenarios, including SAN and NAS convergence, all-level storage convergence, performance and capacity convergence, primary and backup storage convergence, and heterogeneous storage convergence. OceanStor OS helps customers evolve their traditional storage to cloud services in the future.

Summary of Results

SPC-1 Reported Data	
Tested Storage Product (TSP) Name: Huawei OceanStor™ 5600 V3	
Metric	Reported Result
SPC-1 IOPS™	401,005.47
SPC-1 Price-Performance™	\$0.35/SPC-1 IOPS™
Total ASU Capacity	8,504.035 GB
Data Protection Level	Protected 2 (<i>Mirroring</i>)
Total Price	\$141,391.33
Currency Used	U.S. Dollars
Target Country for availability, sales and support	USA

SPC-1 IOPS™ represents the maximum I/O Request Throughput at the 100% load point.

SPC-1 Price-Performance™ is the ratio of **Total Price** to **SPC-1 IOPS™**.

Total ASU (Application Storage Unit) **Capacity** represents the total storage capacity available to be read and written in the course of executing the SPC-1 benchmark.

A **Data Protection Level** of **Protected 2** using *Mirroring* configures two or more identical copies of user data.

Protected 2: *The single point of failure of any component in the configuration will not result in permanent loss of access to or integrity of the SPC-1 Data Repository.*


Total Price includes the cost of the Priced Storage Configuration plus three years of hardware maintenance and software support as detailed on page 17.



Currency Used is formal name for the currency used in calculating the **Total Price** and **SPC-1 Price-Performance™**. That currency may be the local currency of the **Target Country** or the currency of a difference country (*non-local currency*).


The **Target Country** is the country in which the Priced Storage Configuration is available for sale and in which the required hardware maintenance and software support is provided either directly from the Test Sponsor or indirectly via a third-party supplier.

Storage Capacities, Relationships, and Utilization

The following four charts and table document the various storage capacities, used in this benchmark, and their relationships, as well as the storage utilization values required to be reported.

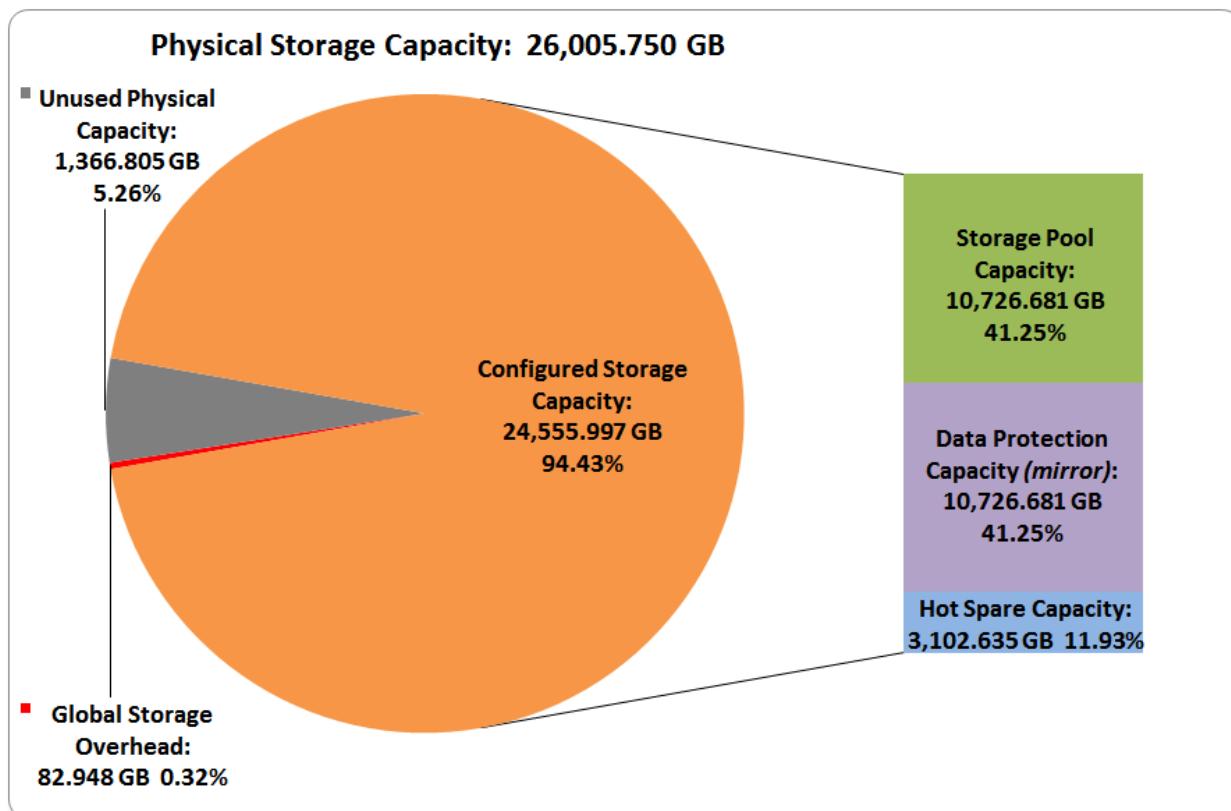

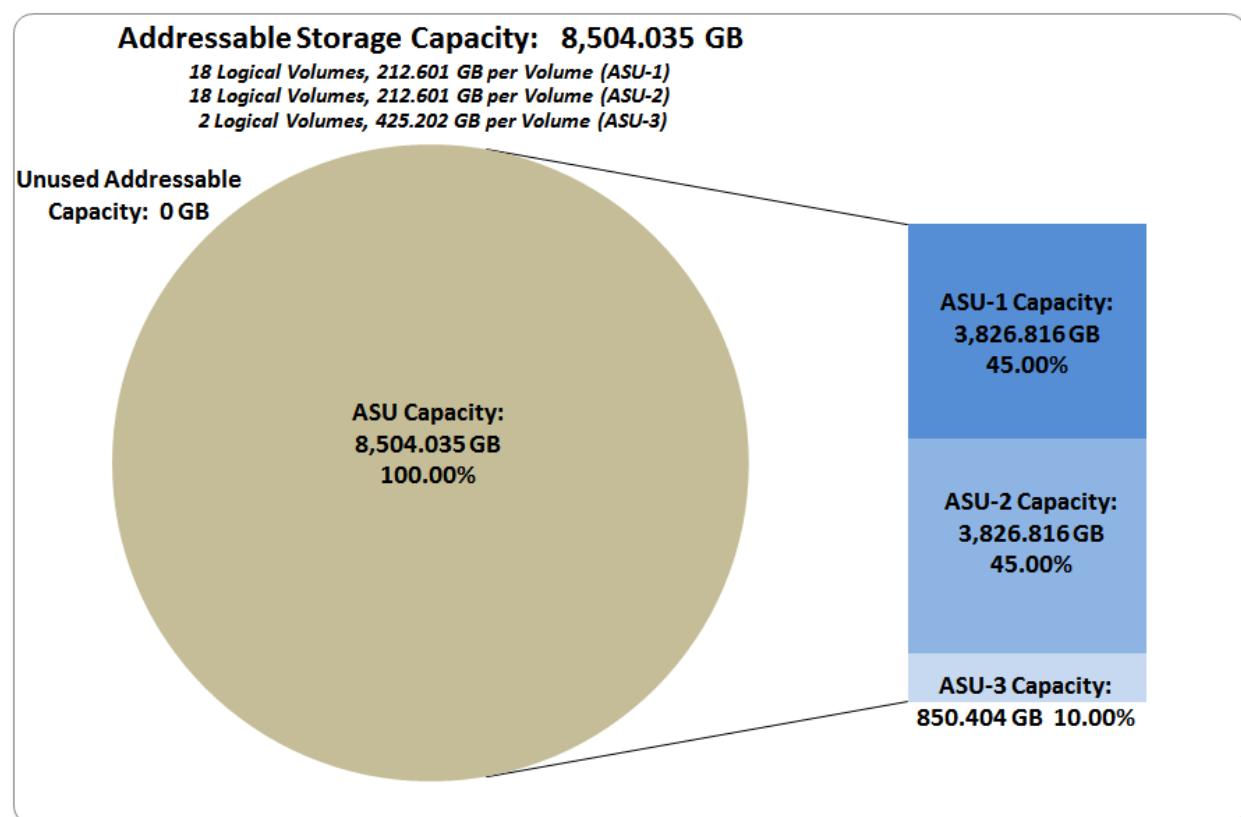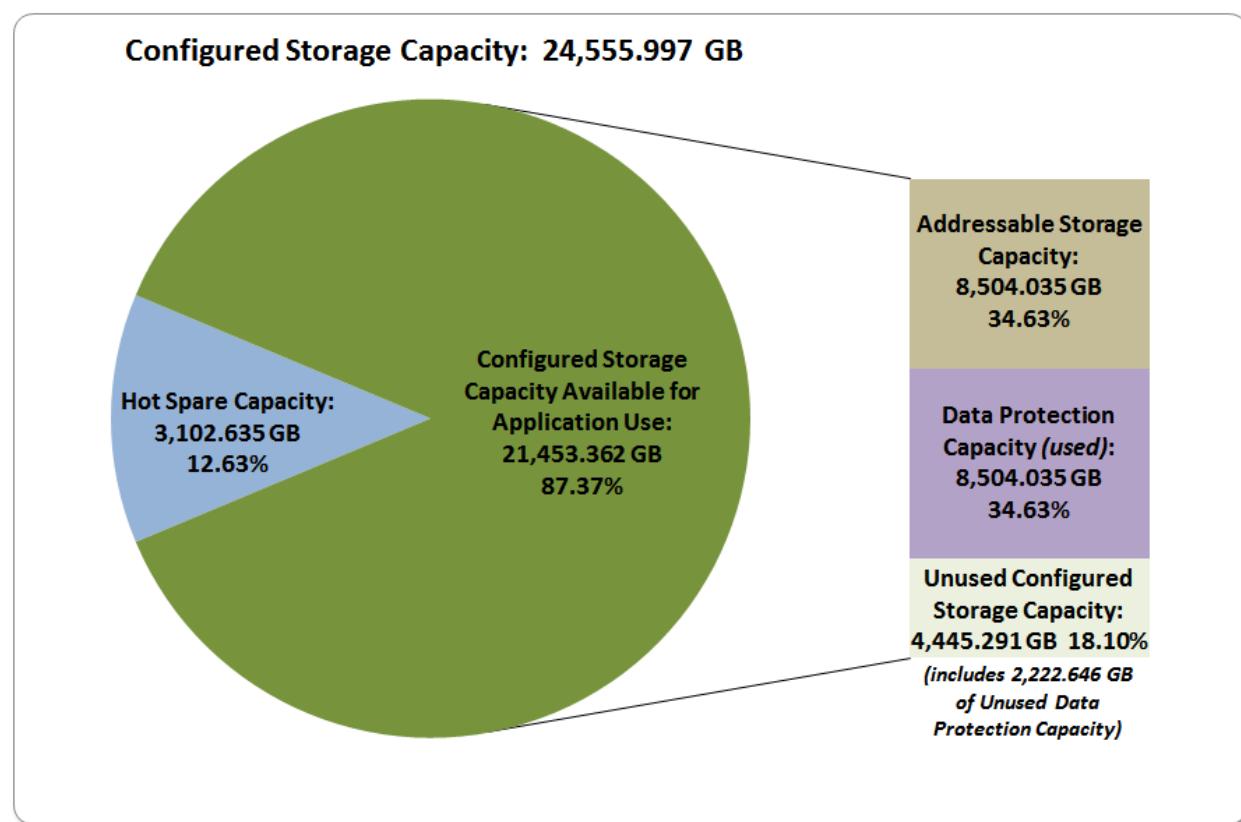

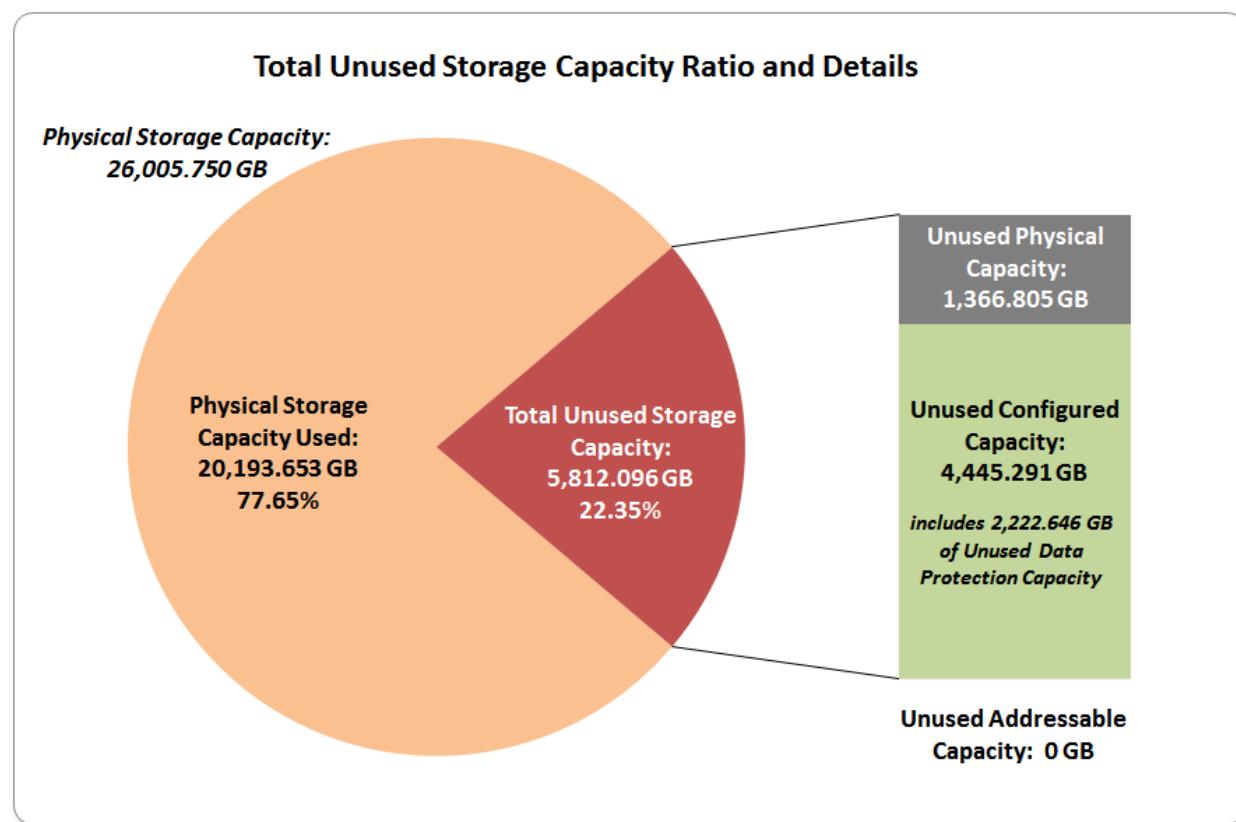

SPC-1 Storage Capacity Utilization	
Application Utilization	32.70%
Protected Application Utilization	65.40%
Unused Storage Ratio	22.35%

Application Utilization: Total ASU Capacity (*8,504.035 GB*) divided by Physical Storage Capacity (*26,005.750 GB*).

Protected Application Utilization: (Total ASU Capacity (*8,504.035 GB*) plus total Data Protection Capacity (*10,726.681 GB*) minus unused Data Protection Capacity (*2,222.646 GB*)) divided by Physical Storage Capacity (*26,005.750 GB*).


Unused Storage Ratio: Total Unused Capacity (*5,812,096 GB*) divided by Physical Storage Capacity (*26,005.750 GB*) and may not exceed 45%.

Detailed information for the various storage capacities and utilizations is available on pages 32-33.

Response Time – Throughput Curve

The Response Time-Throughput Curve illustrates the Average Response Time (milliseconds) and I/O Request Throughput at 100%, 95%, 90%, 80%, 50%, and 10% of the workload level used to generate the SPC-1 IOPS™ metric.

The Average Response Time measured at any of the above load points cannot exceed 30 milliseconds or the benchmark measurement is invalid.

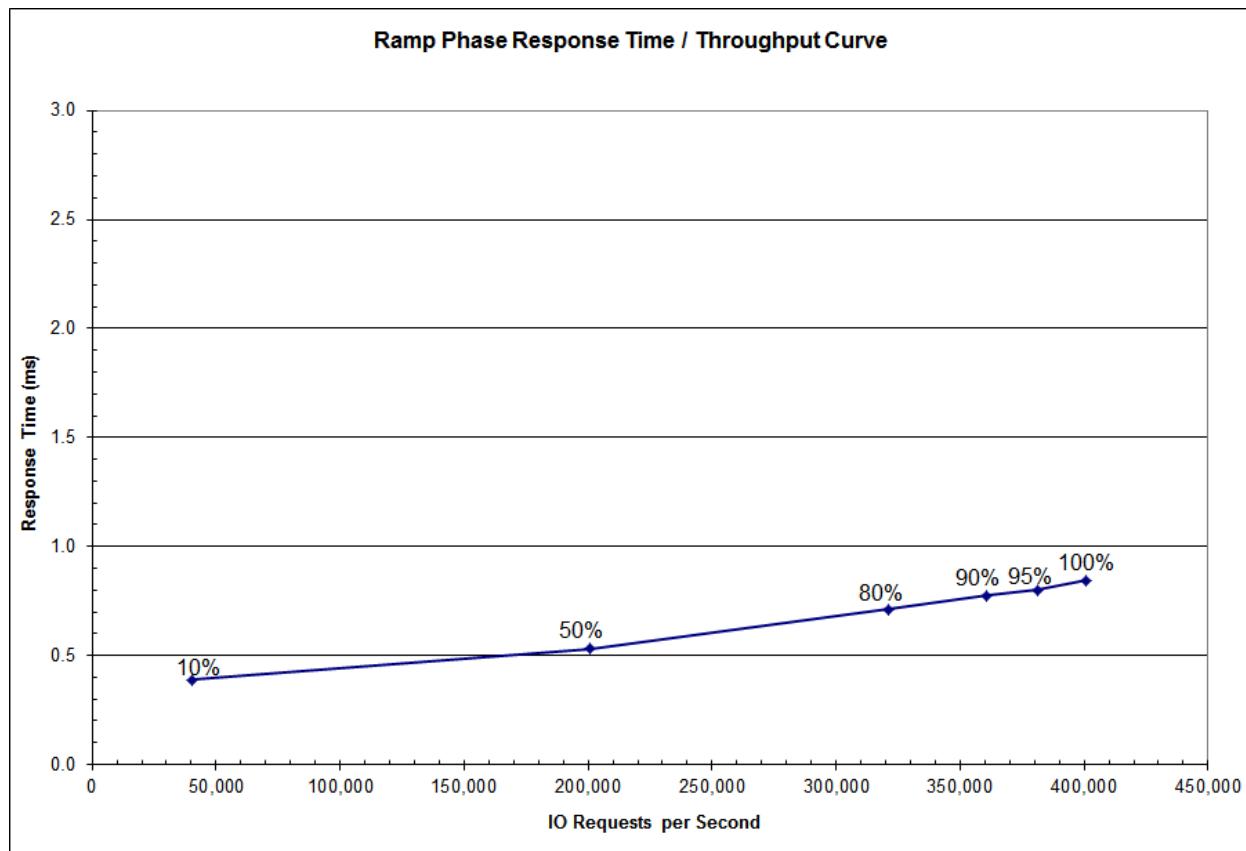

Response Time – Throughput Data

	10% Load	50% Load	80% Load	90% Load	95% Load	100% Load
I/O Request Throughput	40,104.42	200,523.84	320,814.71	360,918.61	380,979.14	401,005.47
Average Response Time (ms):						
All ASUs	0.39	0.53	0.71	0.78	0.80	0.84
ASU-1	0.38	0.57	0.77	0.84	0.87	0.91
ASU-2	0.40	0.59	0.80	0.87	0.90	0.95
ASU-3	0.40	0.42	0.54	0.59	0.60	0.65
Reads	0.39	0.72	0.99	1.08	1.14	1.17
Writes	0.38	0.41	0.53	0.58	0.58	0.63

Priced Storage Configuration Pricing

No.	Model	Description	Qty.	Unit Price (USD)	Total Price (USD)
1	Phase				
1	Location				
1.1	OceanStor 5600 V3 Storage System				
1.1.1	Engine				
	5600V3-128G-AC	5600 V3(3U,Dual Ctrl,AC,128GB,SPE62C0300)	2	16,804.32	33,608.64
1.1.2	Expand Interface Module				
	SMARTIO8FC	4 port SmartIO I/O module(SFP+,8Gb FC)	8	665.04	5,320.32
	SMARTIO10ETH	4 port SmartIO I/O module(SFP+,10Gb Eth/FCoE(VN2VF)/Scale-out)	4	1,310.16	5,240.64
	LPU4S12V3	4 port 4*12Gb SAS I/O module(MiniSAS HD)	8	992.64	7,941.12
1.1.3	Disk Components				
	SSDM-400G2S-A1	SSD Midrange 400GB 2.5" SAS 6G Disk Unit	64	710.40	45,465.60
1.1.4	Disk Enclosure				
	DAE22525U2-1-AC	Disk Enclosure(2U,AC,2.5",Expanding Module,25 Disk Slots,without Disk Unit, DAE22525U2)	4	2,116.80	8,467.20
1.1.5	Installation Material				
	SN2F01FCPC	Patch Cord,DLC/PC,DLC/PC,Multi-mode,3m,A1a.2,2mm,OM3 bending insensitive	40	11.00	440.00
1.1.6	HBA				
	N8GHBA000	QLOGIC QLE2562 HBA Card,PCIE,8Gbps DualPort ,Fiber Channel Multimode LC Optic Interface,English Manual, No Drive CD	16	1,000.00	16,000.00
1.1.7	Storage Software				
	LIC-5600V3-BS	Basic Software License for Block(Include Device Management,SmartThin,SmartMulti-tenant,SmartMigration,SmartErase,SmartMotion,Cloud Service)	1	1,970.16	1,970.16
	LIC-5500V3-PATH	OceanStor HW UltraPath Software License	1	945.60	945.60
Total of Product					125,399.28
1.1.8	Maintenance Support Service				
	02359805-88134ULJ-3	5600 V3(3U,Dual Ctrl,AC,128GB,SPE62C0300)-Warranty Upgrade To Hi-Care Onsite Premier 24x7x4H Engineer Onsite Service-3Year(s)	2	3,790.01	7,580.02
	02359806-88134ULJ-3	Disk Enclosure(2U,AC,2.5",Expanding Module,25 Disk Slots,without Disk Unit,DAE22525U2)-Warranty Upgrade To Hi-Care Onsite Premier 24x7x4H Engineer Onsite Service-3Year(s)	3	2,440.01	7,320.03
	88032QRN-88134UHK-3	OceanStor HW UltraPath Software License-Hi-Care Application Software Upgrade Support Service-3Year(s)	1	354.00	354.00
	88032QRA-88134UHK-3	Basic Software License for Block(Include Device Management,SmartThin,SmartMulti-tenant,SmartMigration,SmartErase,SmartMotion,Cloud Service)-Hi-Care Application Software Upgrade Support Service-3Year(s)	1	738.00	738.00
Total of Service (3 years)					15,992.05
Total Price					141,391.33
Notes:Hi-Care Premier On-Site Service include: 7*24 Technical Assistance Center Access. Access to all new software updates and Online Support. 24*7*4 Hours Onsite Hardware Replacement.					

Huawei Technologies Co., Ltd. only sells its products to third-party resellers, who in turn, sell those products to U.S. customers. The above pricing, which also includes the required three-year maintenance and support, was obtained from one of those third-party resellers. See page [86 \(Appendix F: Third-Party Quotation\)](#) for a copy of the third-party reseller quotation.

The above pricing includes hardware maintenance and software support for three years, 7 days per week, 24 hours per day. The hardware maintenance and software support provides the following:


- Acknowledgement of new and existing problems within four (4) hours.
- Onsite presence of a qualified maintenance engineer or provision of a customer replaceable part within four (4) hours of the above acknowledgement for any hardware failure that results in an inoperative Price Storage Configuration that can be remedied by the repair or replacement of a Priced Storage Configuration component.

Differences between the Tested Storage Configuration (TSC) and Priced Storage Configuration

There were no differences between the Tested Storage Configuration and the Priced Storage Configuration.

Priced Storage Configuration Diagram

16 – QLogic dual-ported QLE2562 FC HBAs

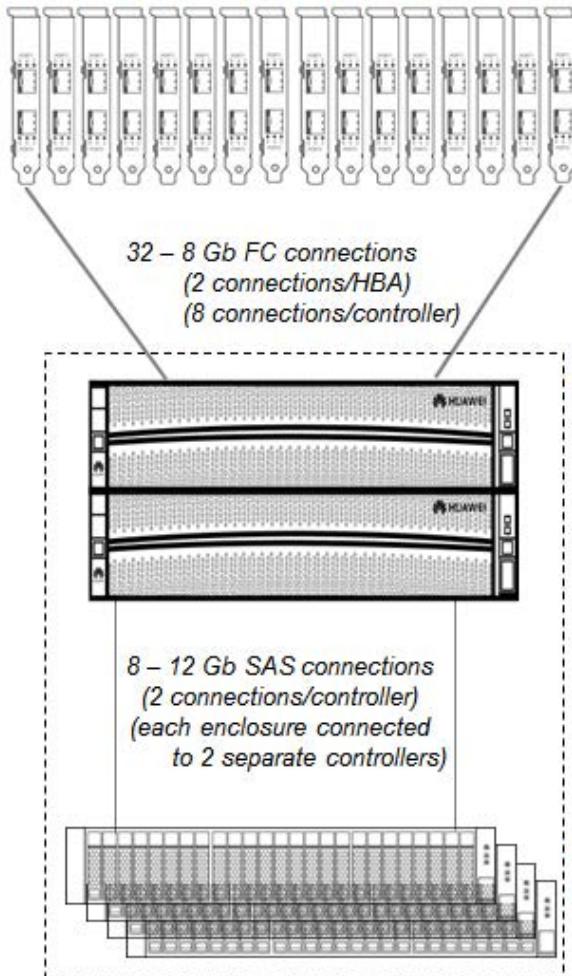

2 – 3U System Enclosures

2 – Engines

(1 Engine per System Enclosure)

4 – Active-Active Controllers

(2 Controllers per Engine)

256 GB cache (64 GB per Controller)

4 – 4-port 10Gb Smart I/O modules
(Eth/FCoE) (1 module per controller)

8 – 4-port 8Gb Smart I/O modules (FC)
(2 modules per controller)

8 – 4-port 12Gbps SAS I/O Modules
(2 modules per controller)

4 – 2U disk enclosures

64 – 400GB 2.5" SSD drives
(16 SSDs per disk enclosure)

Huawei OceanStor™ 5600 V3

Priced Storage Configuration Components

Priced Storage Configuration
OceanStor UltraPath
16 – QLogic QLE2562 dual-port, 8 Gbps, FC HBAs <i>(8 HBAs per server)</i>
Huawei OceanStor™ 5600 V3
2 – 3U System Enclosures
2 – Engines (<i>CTE0 and CTE1</i>) <i>(one Engine per System Enclosure)</i>
4 – Active-Active Controllers (<i>0A, 0B, 1A and 1B</i>) <i>(two Controllers per Engine)</i> each controller includes:
64 GB cache (<i>256 GB total</i>)
1 – 4-port 10Gb Smart I/O modules (<i>Eth/FCoE</i>) <i>(used for inter-controller connectivity)</i> <i>(4 modules total, 4 ports per controller)</i> <i>(16 ports total and used)</i>
2 – 4-port 8Gb Smart I/O module (<i>FC</i>) <i>(8 modules total, 8 ports per controller)</i> <i>(32 ports total and used)</i>
2 – 4-port 12Gbps SAS I/O Modules <i>(8 modules total, 8 ports per controller)</i> <i>(32 ports total, 8 ports used)</i>
4 – 2U Disk Enclosures (<i>DAE000, DAE040, DAE100, DAE140</i>) <i>(each enclosure connected to two separate controllers)</i>
64 – 400 GB, 2.5" SSD drives (<i>16 SSDs per disk enclosure</i>)

Engine, Controller, Eth/FCoE module/active port relationships and Controller-to-Controller Eth/FCoE connection details, used in the Benchmark Configuration, are listed on pages [25-27](#).

Engine, Controller, SAS module/active port relationships and Controller/Disk Enclosure SAS connection details, used in the Benchmark Configuration, are listed on pages [27-28](#).

In each of the following sections of this document, the appropriate Full Disclosure Report requirement, from the SPC-1 benchmark specification, is stated in italics followed by the information to fulfill the stated requirement.

CONFIGURATION INFORMATION

Benchmark Configuration (BC)/Tested Storage Configuration (TSC) Diagram

Clause 9.4.3.4.1

A one page Benchmark Configuration (BC)/Tested Storage Configuration (TSC) diagram shall be included in the FDR...

The Benchmark Configuration (BC)/Tested Storage Configuration (TSC) is illustrated on page [22 \(Benchmark Configuration/Tested Storage Configuration Diagram\)](#).

Storage Network Configuration

Clause 9.4.3.4.1

...

5. *If the TSC contains network storage, the diagram will include the network configuration. If a single diagram is not sufficient to illustrate both the Benchmark Configuration and network configuration in sufficient detail, the Benchmark Configuration diagram will include a high-level network illustration as shown in Figure 9-8. In that case, a separate, detailed network configuration diagram will also be included as described in Clause 9.4.3.4.2.*

Clause 9.4.3.4.2

If a storage network was configured as a part of the Tested Storage Configuration and the Benchmark Configuration diagram described in Clause 9.4.3.4.1 contains a high-level illustration of the network configuration, the Executive Summary will contain a one page topology diagram of the storage network as illustrated in Figure 9-9.


The Tested Storage Configuration (TSC) was configured with direct-attached storage.

Host System(s) and Tested Storage Configuration (TSC) Table of Components

Clause 9.4.3.4.3


The FDR will contain a table that lists the major components of each Host System and the Tested Storage Configuration (TSC).

The Host System(s) and TSC table of components may be found on page [23 \(Host System and Tested Storage Configuration Components\)](#).

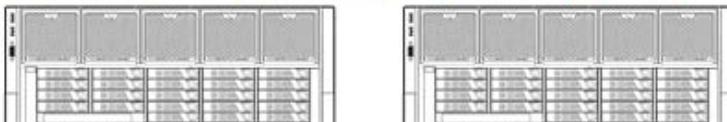
Benchmark Configuration/Tested Storage Configuration Diagram**2 – Huawei FusionServer RH5885 V3 servers**

16 – QLogic dual-ported QLE2562 FC HBAs
(8 HBAs per server)

32 – 8 Gb FC connections
(2 connections/HBA)
(8 connections/controller)

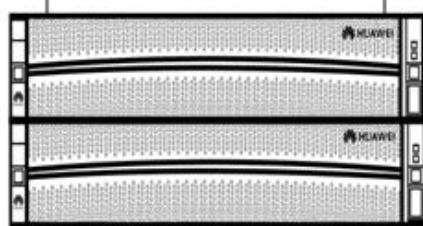

8 – 12 Gb SAS connections
(2 connections/controller)
(each enclosure connected to 2 separate controllers)

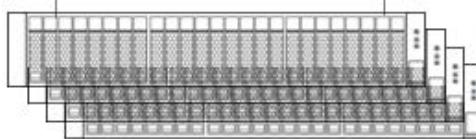**2 – 3U System Enclosures****2 – Engines**

(1 Engine per System Enclosure)

4 – Active-Active Controllers
(2 Controllers per Engine)

256 GB cache (64 GB per Controller)

4 – 4-port 10Gb Smart I/O modules
(Eth/FCoE) (1 module per controller)

8 – 4-port 8Gb Smart I/O modules (FC)
(2 modules per controller)

8 – 4-port 12Gbps SAS I/O Modules
(2 modules per controller)

4 – 2U disk enclosures

64 – 400GB 2.5" SSD drives
(16 SSDs per disk enclosure)

Huawei OceanStor™ 5600 V3

Host System and Tested Storage Configuration Components

Host System
2 – Huawei FusionServer RH5885 V3 servers , each with: 4 – Intel® Xeon® 2.00 GHz processor E7-4820 V2 each with 8 cores, 16 MB cache 512 GB main memory Red Hat Enterprise Linux Server release 7.0 x86_64 PCIe
Tested Storage Configuration
OceanStor UltraPath
16 – QLogic QLE2562 dual-port, 8 Gbps, FC HBAs (8 HBAs per server)
Huawei OceanStor™ 5600 V3
2 – 3U System Enclosures 2 – Engines (<i>CTE0 and CTE1</i>) <i>(one Engine per System Enclosure)</i> 4 – Active-Active Controllers (<i>0A, 0B, 1A and 1B</i>) <i>(two Controllers per Engine)</i> each controller includes: 64 GB cache (<i>256 GB total</i>) 1 – 4-port 10Gb Smart I/O modules (<i>Eth/FCoE</i>) <i>(used for inter-controller connectivity)</i> <i>(4 modules total, 4 ports per controller)</i> <i>(16 ports total and used)</i> 2 – 4-port 8Gb Smart I/O module (<i>FC</i>) <i>(8 modules total, 8 ports per controller)</i> <i>(32 ports total and used)</i> 2 – 4-port 12Gbps SAS I/O Modules <i>(8 modules total, 8 ports per controller)</i> <i>(32 ports total, 8 ports used)</i> 4 – 2U Disk Enclosures (<i>DAE000, DAE040, DAE100, DAE140</i>) <i>(each enclosure connected to two separate controllers)</i> 64 – 400 GB, 2.5" SSD drives (<i>16 SSDs per disk enclosure</i>)

Host System, HBA, Engine, Controller, FC Host Port Module details and Host System HBA/Host Port FC connections are listed on page [24](#).

Engine, Controller, Eth/FCoE module/active port relationships and Controller-to-Controller Eth/FCoE connection details are listed on pages [25-27](#).

Engine, Controller, SAS module/active port relationships and Controller/Disk Enclosure SAS connection details are listed on pages [27-28](#).

Benchmark Configuration/Tested Storage Configuration Connections

Host System, FC HBA, Engine, Controller, FC Host Port Module/Ports

The Benchmark Configuration/Tested Storage Configuration includes:

- 2 Host Systems: **Host System 1** and **Host System 2**
- 16 FC HBAs (*2 ports per HBA, 32 ports total*)
 - 8 FC HBAs per Host System: **HBA0 – HBA7** (*arbitrary names for identification*)
 - 16 ports per Host System

Huawei OceanStor™ 5600 V3

- 2 Engines: **CTE0** and **CTE1**
 - 4 Controllers: **0A, 0B, 1A** and **1B**
 - 2 Controllers per Engine: **CTE0.0A** and **CTE0.0B**; **CTE1.1A** and **CTE1.1B**
 - 8 FC Host Port Modules:
 - CTE0.A4, CTE0.A7, CTE0.B4, CTE0.B7, CTE1.A4, CTE1.A7, CTE1.B4** and **CTE1.B7**
- 4 ports per Module (P0 – P3), 2 Modules per Controller:
- CTE0.0A:** **CTE0.A4.P0 – P3, CTE0.A7.P0 – P3**
 - CTE0.0B:** **CTE0.B4.P0 – P3, CTE0.B7.P0 – P3**
 - CTE1.1A:** **CTE1.A4.P0 – P3, CTE1.A7.P0 – P3**
 - CTE1.1B:** **CTE1.B4.P0 – P3, CTE1.B7.P0 – P3**

Host System to Controller Host Port FC Connections

Each Host System has 4 FC HBA connections to each controller, as described below, which utilizes all 32 HBA and controller FC port.

- **Host System 1**
 - **HBA0:** 2 HBA ports connected to any 2 ports in controller **0A**, FC module **CTE0.A4**
 - **HBA1:** 2 HBA ports connected to any 2 ports in controller **0A**, FC module **CTE0.A7**
 - **HBA2:** 2 HBA ports connected to any 2 ports in controller **0B**, FC module **CTE0.B4**
 - **HBA3:** 2 HBA ports connected to any 2 ports in controller **0B**, FC module **CTE0.B7**
 - **HBA4:** 2 HBA ports connected to any 2 ports in controller **1A**, FC module **CTE1.A4**
 - **HBA5:** 2 HBA ports connected to any 2 ports in controller **1A**, FC module **CTE1.A7**
 - **HBA6:** 2 HBA ports connected to any 2 ports in controller **1B**, FC module **CTE1.B4**
 - **HBA7:** 2 HBA ports connected to any 2 ports in controller **1B**, FC module **CTE1.B7**
- **Host System 2**
 - **HBA0:** 2 HBA ports connected to any 2 ports in controller **0A**, FC module **CTE0.A4**
 - **HBA1:** 2 HBA ports connected to any 2 ports in controller **0A**, FC module **CTE0.A7**
 - **HBA2:** 2 HBA ports connected to any 2 ports in controller **0B**, FC module **CTE0.B4**
 - **HBA3:** 2 HBA ports connected to any 2 ports in controller **0B**, FC module **CTE0.B7**
 - **HBA4:** 2 HBA ports connected to any 2 ports in controller **1A**, FC module **CTE1.A4**
 - **HBA5:** 2 HBA ports connected to any 2 ports in controller **1A**, FC module **CTE1.A7**

- **HBA6:** 2 HBA ports connected to any 2 ports in controller **1B**, FC module **CTE1.B4**
- **HBA7:** 2 HBA ports connected to any 2 ports in controller **1B**, FC module **CTE1.B7**

Engine, Controller, Eth/FCoE Module/Active Port Relationships

The relationships between the Engines, Controllers, Eth/FCoE Modules/Active Ports are listed below and illustrated in the following table.

- 2 Engines: **CTE0** and **CTE1**
- 4 Controllers: **0A**, **0B**, **1A** and **1B**
2 Controllers per Engine: **CTE0.0A** and **CTE0.0B**; **CTE1.1A** and **CTE1.1B**
- 4 Eth/FCoE Modules:
CTE0.A3, **CTE0.B3**, **CTE1.A3** and **CTE1.B3**
1 Module per Controller, 4 ports per Module (**P0 – P3**):
CTE0.0A: **CTE0.A3.P0 – P3**
CTE0.0B: **CTE0.B3.P0 – P3**
CTE1.1A: **CTE1.A3.P0 – P3**
CTE1.1B: **CTE1.B3.P0 – P3**

Engine	Controller	Eth/FCoE Module	Active Port
CTE0	0A	CTE0.A3	CTE0.A3.P0
			CTE0.A3.P1
			CTE0.A3.P2
			CTE0.A3.P3
	0B	CTE0.B3	CTE0.B3.P0
			CTE0.B3.P1
			CTE0.B3.P2
			CTE0.B3.P3
CTE1	1A	CTE1.A3	CTE1.A3.P0
			CTE1.A3.P1
	1B	CTE1.B3	CTE1.A3.P2
			CTE1.A3.P3
	1B	CTE1.B3	CTE1.B3.P0
			CTE1.B3.P1
			CTE1.B3.P2
			CTE1.B3.P3

Controller-to-Controller Eth/FCoE Connections

The following table and diagram documents and illustrates the Eth/FCoE connections between each Controller to scale-out from two to four Controllers.

Controller-to-Controller Eth/FCoE Connections


Engine CTE1	Engine CTE0							
	Controller 0A				Controller 0B			
	CTE0.A3.P0	CTE0.A3.P1	CTE0.A3.P2	CTE0.A3.P3	CTE0.B3.P0	CTE0.B3.P1	CTE0.B3.P2	CTE0.B3.P3
Controller 1A								
CTE1.A3.P0	connection							
CTE1.A3.P1		connection						
CTE1.A3.P2						connection		
CTE1.A3.P3							connection	
Controller 1B								
CTE1.B3.P0					connection			
CTE1.B3.P1						connection		
CTE1.B3.P2			connection					
CTE1.B3.P3				connection				

Engine CTE0: Controller 0A, Eth/FCoE Module CTE0.A3 Ports P0-P3

Controller 0B, Eth/FCoE Module CTE0.B3 Ports P0-P3

Engine CTE1: Controller 1A, Eth/FCoE Module CTE1.A3 Ports P0-P3

Controller 1B, Eth/FCoE Module CTE1.B3 Ports P0-P3

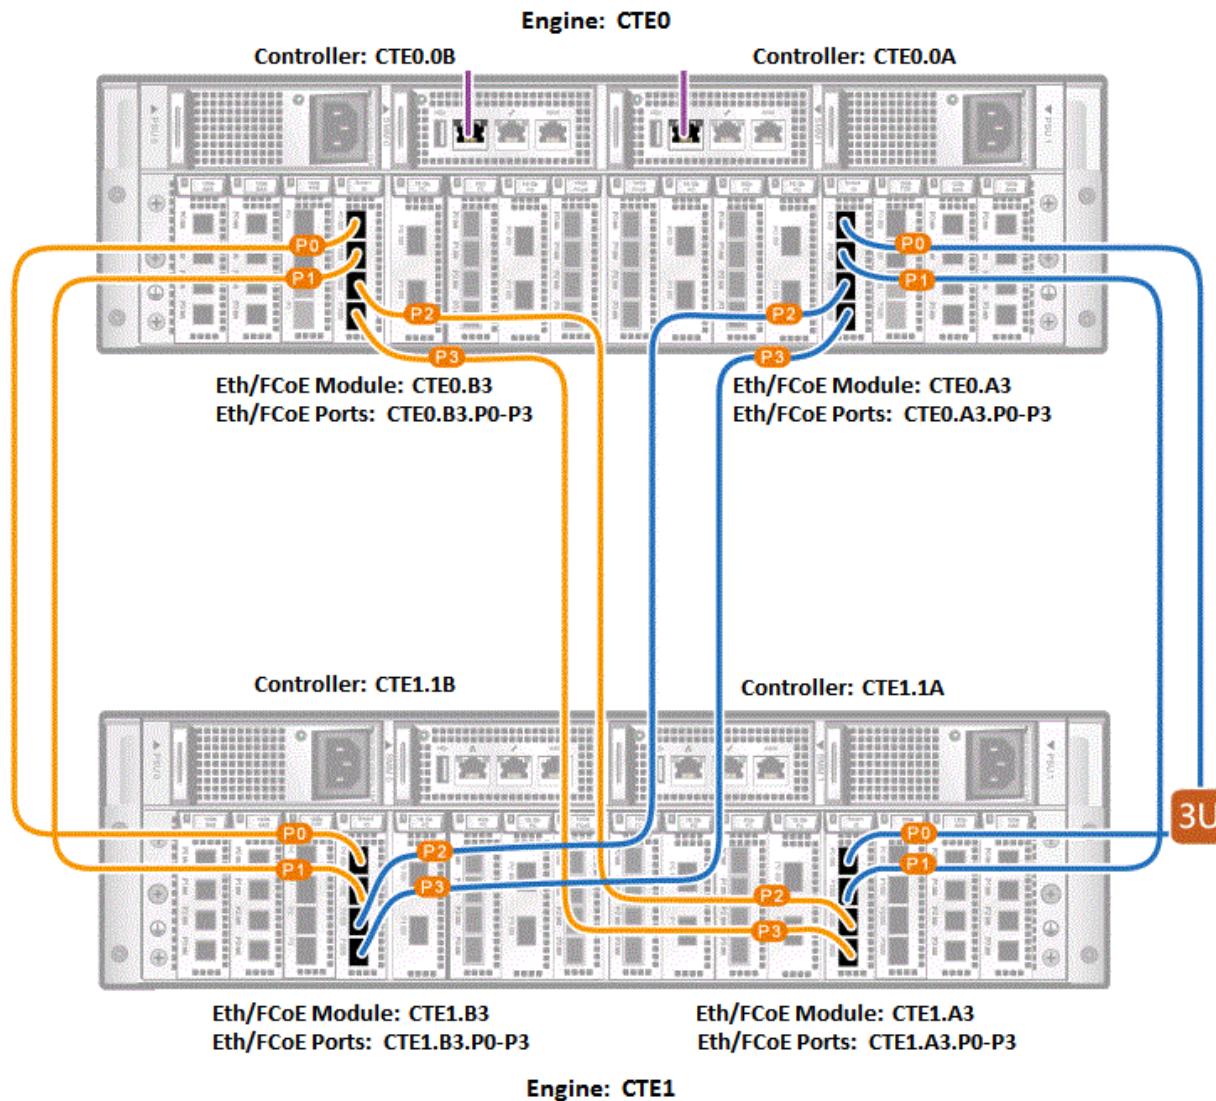Controller to Controller Eth/FCoE Connections (*continued*)

Engine, Controller and SAS Module/Active Port Relationships

The relationship between the Engines, Controllers and SAS Modules/Active Ports are listed below and illustrated in the following table.

- 2 Engines: **CTE0** and **CTE1**
- 4 Controllers: **0A, 0B, 1A** and **1B**
2 Controllers per Engine: **CTE0.0A** and **CTE0.0B**; **CTE1.1A** and **CTE1.1B**
- 8 SAS Modules:
CTE0.A0, CTE0.A1, CTE0.B0, CTE0.B1, CTE1.A0, CTE1.A1, CTE1.B0 and **CTE1.B1**
2 Modules per Controller, 4 ports per Module (**P0 – P3**):
CTE0.0A: **CTE0.A0.P0 – P3, CTE0.A1.P0 – P3**
CTE0.0B: **CTE0.B0.P0 – P3, CTE0.B1.P0 – P3**
CTE1.1A: **CTE1.A0.P0 – P3, CTE1.A1.P0 – P3**
CTE1.1B: **CTE1.B0.P0 – P3, CTE1.B1.P0 – P3**
- 4 Disk Enclosures: **DAE000, DAE040, DAE100** and **DAE140**
4 SAS Ports per Enclosure: **A.PRI, A.EXP, B.PRI**, and **B.PRI**

Engine	Controller	SAS Module	Active Port
CTE0	0A	A0	CTE0.A0.P0
		A1	CTE0.A1.P0
	0B	B0	CTE0.B0.P0
		B1	CTE0.B1.P0
CTE1	1A	A0	CTE1.A0.P0
		A1	CTE1.A1.P0
	1B	B0	CTE1.B0.P0
		B1	CTE1.B1.P0

Controller/Disk Enclosure SAS Connections

The following table documents the connection between each Controller's active SAS port and the corresponding Disk Enclosure's active SAS port.

Controller/Disk Enclosure SAS Connections

Disk Enclosures and Active Ports	Engines, Controllers and Active SAS Ports							
	Engine CTE0				Engine CTE1			
	Controller 0A		Controller 0B		Controller 1A		Controller 1B	
	CTE0.A0.P0	CTE0.A1.P0	CTE0.B0.P0	CTE0.B1.P0	CTE1.A0.P0	CTE1.A1.P0	CTE1.B0.P0	CTE1.B1.P0
DAE000								
DAE000.A.PRI	connection							
DAE000.B.PRI			connection					
DAE040								
DAE040.A.PRI		connection						
DAE040.B.PRI				connection				
DAE100								
DAE100.A.PRI					connection			
DAE100.B.PRI						connection		
DAE140								
DAE140.A.PRI						connection		
DAE140.B.PRI							connection	

Customer Tunable Parameters and Options

Clause 9.4.3.5.1

All Benchmark Configuration (BC) components with customer tunable parameter and options that have been altered from their default values must be listed in the FDR. The FDR entry for each of those components must include both the name of the component and the altered value of the parameter or option. If the parameter name is not self-explanatory to a knowledgeable practitioner, a brief description of the parameter's use must also be included in the FDR entry.

[Appendix B: Customer Tunable Parameters and Options](#) on page [73](#) contains the customer tunable parameters and options that have been altered from their default values for this benchmark.

Tested Storage Configuration (TSC) Description

Clause 9.4.3.5.2

The FDR must include sufficient information to recreate the logical representation of the TSC. In addition to customer tunable parameters and options (Clause 4.2.4.5.3), that information must include, at a minimum:

- *A diagram and/or description of the following:*
 - *All physical components that comprise the TSC. Those components are also illustrated in the BC Configuration Diagram in Clause 9.2.4.4.1 and/or the Storage Network Configuration Diagram in Clause 9.2.4.4.2.*
 - *The logical representation of the TSC, configured from the above components that will be presented to the Workload Generator.*
- *Listings of scripts used to create the logical representation of the TSC.*
- *If scripts were not used, a description of the process used with sufficient detail to recreate the logical representation of the TSC.*

[Appendix C: Tested Storage Configuration \(TSC\) Creation](#) on page [74](#) contains the detailed information that describes how to create and configure the logical TSC.

SPC-1 Workload Generator Storage Configuration

Clause 9.4.3.5.3

The FDR must include all SPC-1 Workload Generator storage configuration commands and parameters.

The SPC-1 Workload Generator storage configuration commands and parameters for this measurement appear in [Appendix D: SPC-1 Workload Generator Storage Commands and Parameters](#) on page [80](#).

ASU Pre-Fill

Clause 5.3.3

Each of the three SPC-1 ASUs (ASU-1, ASU-2 and ASU-3) is required to be completely filled with specified content prior to the execution of audited SPC-1 Tests. The content is required to consist of random data pattern such as that produced by an SPC recommended tool.

The configuration file used to complete the required ASU pre-fill appears in [Appendix D: SPC-1 Workload Generator Storage Commands and Parameters](#) on page [80](#).

SPC-1 DATA REPOSITORY

This portion of the Full Disclosure Report presents the detailed information that fully documents the various SPC-1 storage capacities and mappings used in the Tested Storage Configuration. [SPC-1 Data Repository Definitions](#) on page [69](#) contains definitions of terms specific to the SPC-1 Data Repository.

Storage Capacities and Relationships

Clause 9.4.3.6.1

Two tables and four charts documenting the storage capacities and relationships of the SPC-1 Storage Hierarchy (Clause 2.1) shall be included in the FDR. ... The capacity value in each chart may be listed as an integer value, for readability, rather than the decimal value listed in the table below.

SPC-1 Storage Capacities

The Physical Storage Capacity consisted of 25,922.802 GB distributed over 64 solid state drives (SSDs) each with a formatted capacity of 406.340 GB. There was 1,366.805 GB (5.26%) of Unused Storage within the Physical Storage Capacity. Global Storage Overhead consisted of 82.948 GB (0.32%) of the Physical Storage Capacity. There was 4.445.291 GB (18.10%) of Unused Storage within the Configured Storage Capacity. The Total ASU Capacity utilized 100% of the Addressable Storage Capacity resulting in 0.00 GB (0.00%) of Unused Storage within the Addressable Storage Capacity. The Data Protection (*Mirroring*) capacity was 10,726.681 GB of which 8,504.035 GB was utilized. The total Unused Storage capacity was 5,812.096 GB.


Note: The configured Storage Devices may include additional storage capacity reserved for system overhead, which is not accessible for application use. That storage capacity may not be included in the value presented for Physical Storage Capacity.



SPC-1 Storage Capacities		
Storage Hierarchy Component	Units	Capacity
Total ASU Capacity	Gigabytes (GB)	8,504.035
Addressable Storage Capacity	Gigabytes (GB)	8,504.035
Configured Storage Capacity	Gigabytes (GB)	24,555.997
Physical Storage Capacity	Gigabytes (GB)	26,005.750
Data Protection (<i>Mirroring</i>)	Gigabytes (GB)	10,726.681
Required Storage (<i>sparing</i>)	Gigabytes (GB)	3,102.635
Global Storage Overhead	Gigabytes (GB)	82.948
Total Unused Storage	Gigabytes (GB)	5,812.096


SPC-1 Storage Hierarchy Ratios

	Addressable Storage Capacity	Configured Storage Capacity	Physical Storage Capacity
Total ASU Capacity	100.00%	34.63%	32.70%
Required for Data Protection (<i>Mirroring</i>)		43.68%	41.25%
Addressable Storage Capacity		34.63%	32.70%
Required Storage (<i>sparing</i>)		12.63%	11.93%
Configured Storage Capacity			94.43%
Global Storage Overhead			0.32%
Unused Storage:			
Addressable	0.00%		
Configured		18.10%	
Physical			5.26%

SPC-1 Storage Capacity Charts

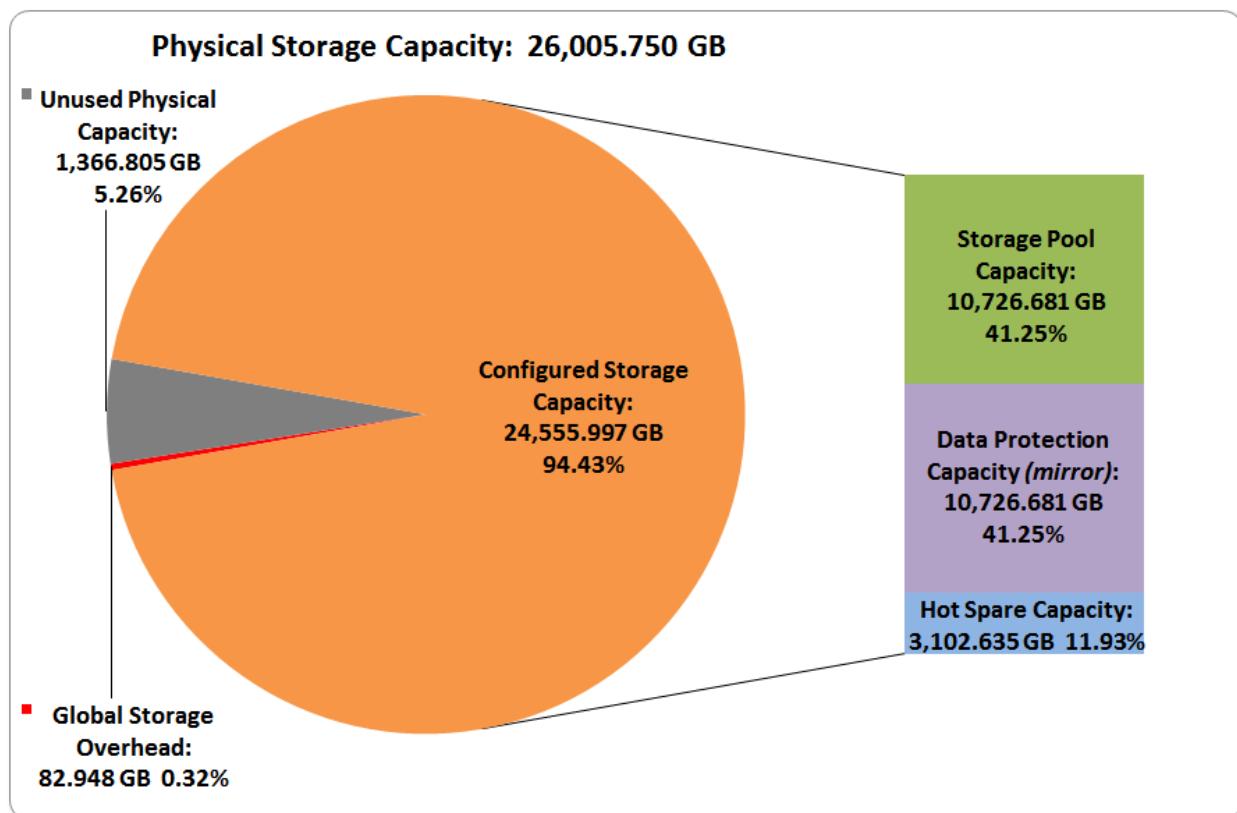

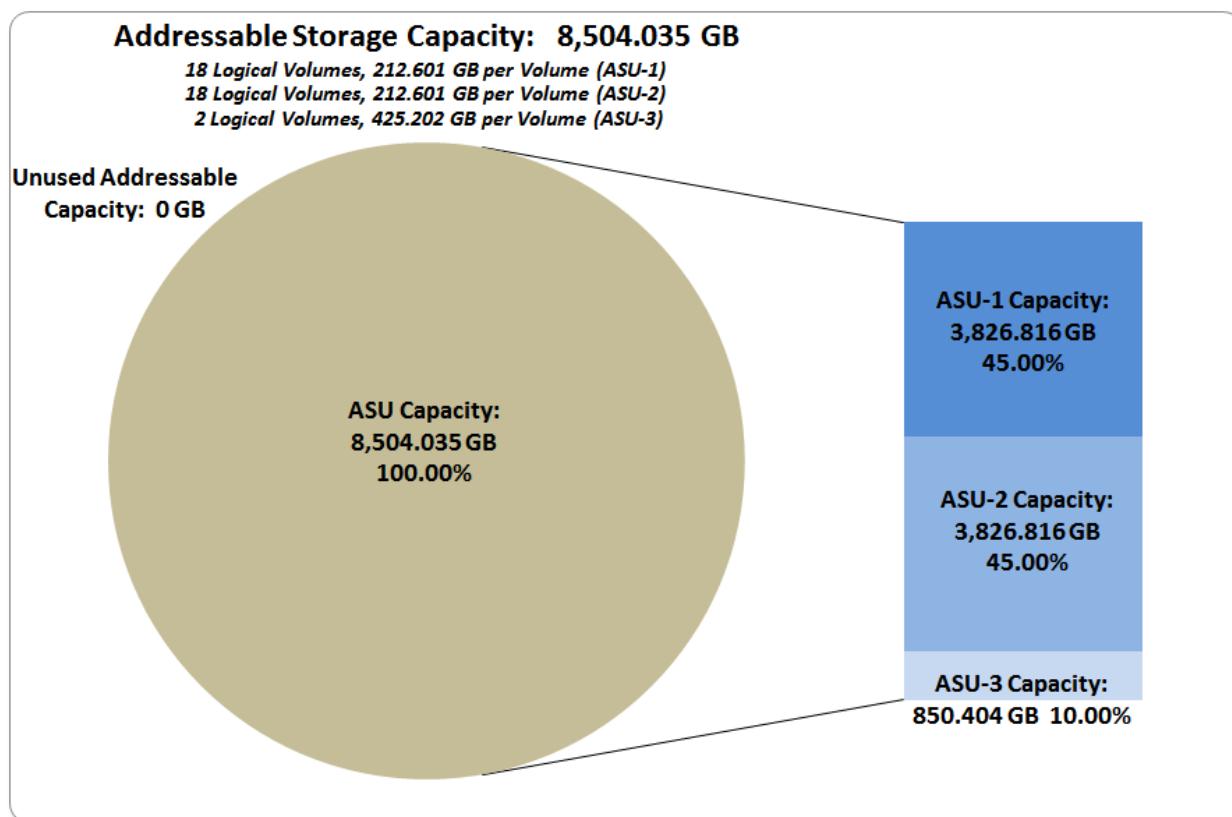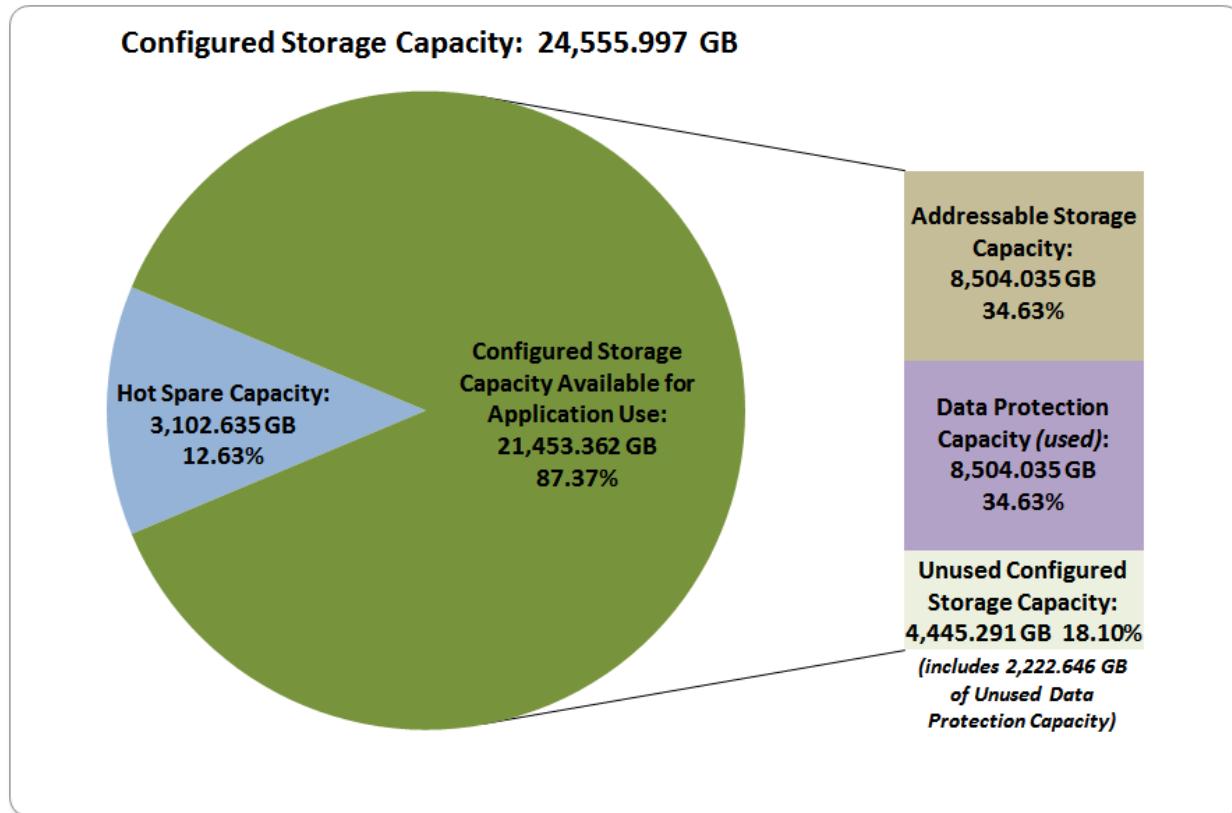

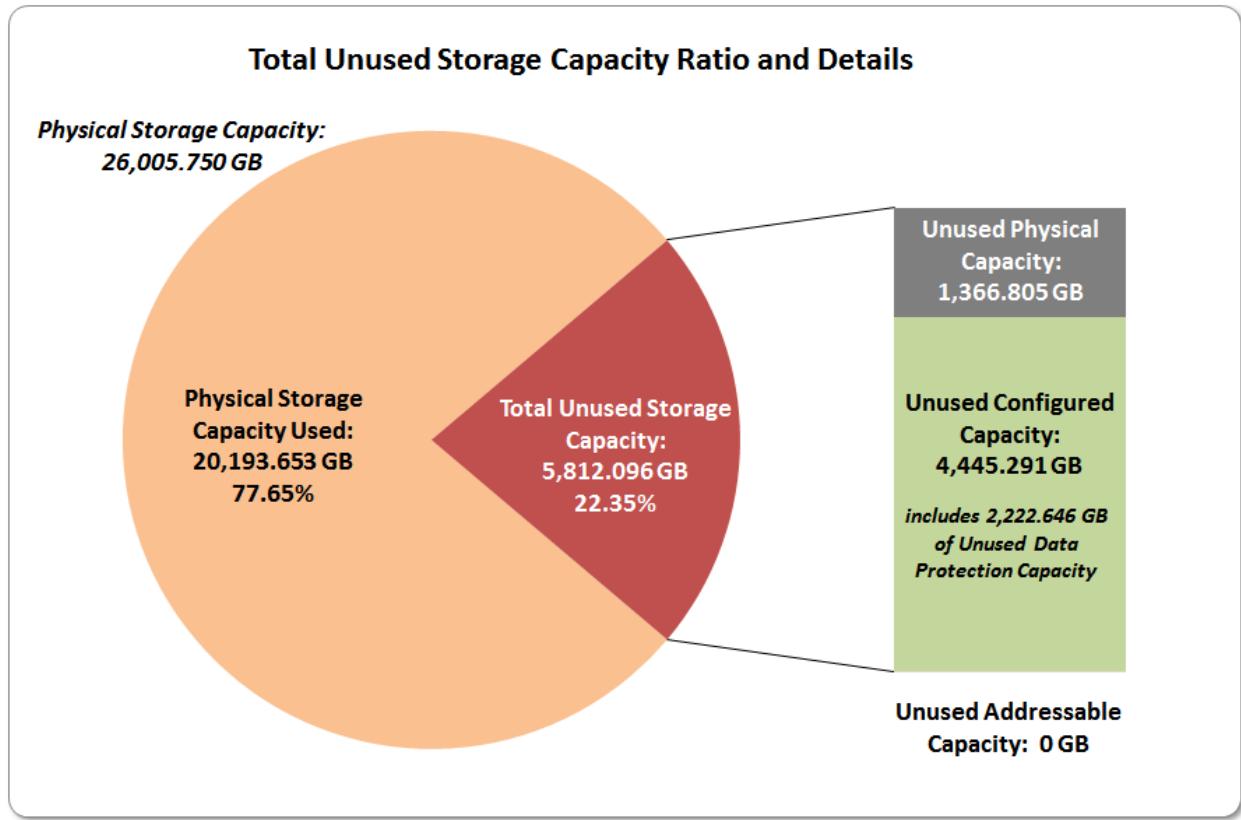

Storage Capacity Utilization

Clause 9.4.3.6.2

The FDR will include a table illustrating the storage capacity utilization values defined for Application Utilization (Clause 2.8.1), Protected Application Utilization (Clause 2.8.2), and Unused Storage Ratio (Clause 2.8.3).

Clause 2.8.1

Application Utilization is defined as Total ASU Capacity divided by Physical Storage Capacity.

Clause 2.8.2

Protected Application Utilization is defined as (Total ASU Capacity plus total Data Protection Capacity minus unused Data Protection Capacity) divided by Physical Storage Capacity.

Clause 2.8.3

Unused Storage Ratio is defined as Total Unused Capacity divided by Physical Storage Capacity and may not exceed 45%.

SPC-1 Storage Capacity Utilization	
Application Utilization	32.70%
Protected Application Utilization	65.40%
Unused Storage Ratio	22.35%

Logical Volume Capacity and ASU Mapping

Clause 9.4.3.6.3

A table illustrating the capacity of each ASU and the mapping of Logical Volumes to ASUs shall be provided in the FDR. ... Logical Volumes shall be sequenced in the table from top to bottom per its position in the contiguous address space of each ASU. The capacity of each Logical Volume shall be stated. ... In conjunction with this table, the Test Sponsor shall provide a complete description of the type of data protection (see Clause 2.4.5) used on each Logical Volume.

Logical Volume Capacity and Mapping	
ASU-1 (3,826.816 GB)	
18 Logical Volumes 212.601 GB per Logical Volume (212.601 GB used per Logical Volume)	
ASU-2 (3,826.816 GB)	
18 Logical Volumes 212.601 GB per Logical Volume (212.601 GB used per Logical Volume)	
ASU-3 (850.404 GB)	
2 Logical Volumes 425.202 GB per Logical Volume (425.202 GB used per Logical Volume)	

The Data Protection Level used for all Logical Volumes was [Protected 2](#) using [Mirroring](#) as described on page [12](#). See “ASU Configuration” in the [IOPS Test Results File](#) for more detailed configuration information.

SPC-1 BENCHMARK EXECUTION RESULTS

This portion of the Full Disclosure Report documents the results of the various SPC-1 Tests, Test Phases, and Test Runs. An [SPC-1 glossary](#) on page 69 contains definitions of terms specific to the SPC-1 Tests, Test Phases, and Test Runs.

Clause 5.4.3

The Tests must be executed in the following sequence: Primary Metrics, Repeatability, and Data Persistence. That required sequence must be uninterrupted from the start of Primary Metrics to the completion of Persistence Test Run 1. Uninterrupted means the Benchmark Configuration shall not be power cycled, restarted, disturbed, altered, or adjusted during the above measurement sequence. If the required sequence is interrupted other than for the Host System/TSC power cycle between the two Persistence Test Runs, the measurement is invalid.

SPC-1 Tests, Test Phases, and Test Runs

The SPC-1 benchmark consists of the following Tests, Test Phases, and Test Runs:

- **Primary Metrics Test**
 - Sustainability Test Phase and Test Run
 - IOPS Test Phase and Test Run
 - Response Time Ramp Test Phase
 - 95% of IOPS Test Run
 - 90% of IOPS Test Run
 - 80% of IOPS Test Run
 - 50% of IOPS Test Run
 - 10% of IOPS Test Run (LRT)
- **Repeatability Test**
 - Repeatability Test Phase 1
 - 10% of IOPS Test Run (LRT)
 - IOPS Test Run
 - Repeatability Test Phase 2
 - 10% of IOPS Test Run (LRT)
 - IOPS Test Run
- **Data Persistence Test**
 - Data Persistence Test Run 1
 - Data Persistence Test Run 2

Each Test is an atomic unit that must be executed from start to finish before any other Test, Test Phase, or Test Run may be executed.

The results from each Test, Test Phase, and Test Run are listed below along with a more detailed explanation of each component.

“Ramp-Up” Test Runs

Clause 5.3.13

In order to warm-up caches or perform the initial ASU data migration in a multi-tier configuration, a Test Sponsor may perform a series of “Ramp-Up” Test Runs as a substitute for an initial, gradual Ramp-Up.

Clause 5.3.13.3

The “Ramp-Up” Test Runs will immediately precede the Primary Metrics Test as part of the uninterrupted SPC-1 measurement sequence.

Clause 9.4.3.7.1

If a series of “Ramp-Up” Test Runs were included in the SPC-1 measurement sequence, the FDR shall report the duration (ramp-up and measurement interval), BSU level, SPC-1 IOPS and average response time for each “Ramp-Up” Test Run in an appropriate table.

There were no “Ramp-Up” Test Runs executed.

Primary Metrics Test – Sustainability Test Phase

Clause 5.4.4.1.1

The Sustainability Test Phase has exactly one Test Run and shall demonstrate the maximum sustainable I/O Request Throughput within at least a continuous eight (8) hour Measurement Interval. This Test Phase also serves to insure that the TSC has reached Steady State prior to reporting the final maximum I/O Request Throughput result (SPC-1 IOPSTM).

Clause 5.4.4.1.2

The computed I/O Request Throughput of the Sustainability Test must be within 5% of the reported SPC-1 IOPSTM result.

Clause 5.4.4.1.4

The Average Response Time, as defined in Clause 5.1.1, will be computed and reported for the Sustainability Test Run and cannot exceed 30 milliseconds. If the Average Response time exceeds that 30-milliseconds constraint, the measurement is invalid.

Clause 9.4.3.7.2

For the Sustainability Test Phase the FDR shall contain:

1. A Data Rate Distribution graph and data table.
2. I/O Request Throughput Distribution graph and data table.
3. A Response Time Frequency Distribution graph and table.
4. An Average Response Time Distribution graph and table.
5. The human readable Test Run Results File produced by the Workload Generator (may be included in an appendix).
6. A listing or screen image of all input parameters supplied to the Workload Generator (may be included in an appendix).
7. The Measured Intensity Multiplier for each I/O stream.
8. The variability of the Measured Intensity Multiplier, as defined in Clause 5.3.13.3.

SPC-1 Workload Generator Input Parameters

The SPC-1 Workload Generator input parameters for the Sustainability, IOPS, Response Time Ramp, Repeatability, and Persistence Test Runs are documented in [Appendix E: SPC-1 Workload Generator Input Parameters](#) on Page [83](#).

Sustainability Test Results File

A link to the test results file generated from the Sustainability Test Run is listed below.


[Sustainability Test Results File](#)

Sustainability – Data Rate Distribution Data (MB/second)

The Sustainability Data Rate table of data is not embedded in this document due to its size. The table is available via the following URL:

[Sustainability Data Rate Table](#)

Sustainability – Data Rate Distribution Graph

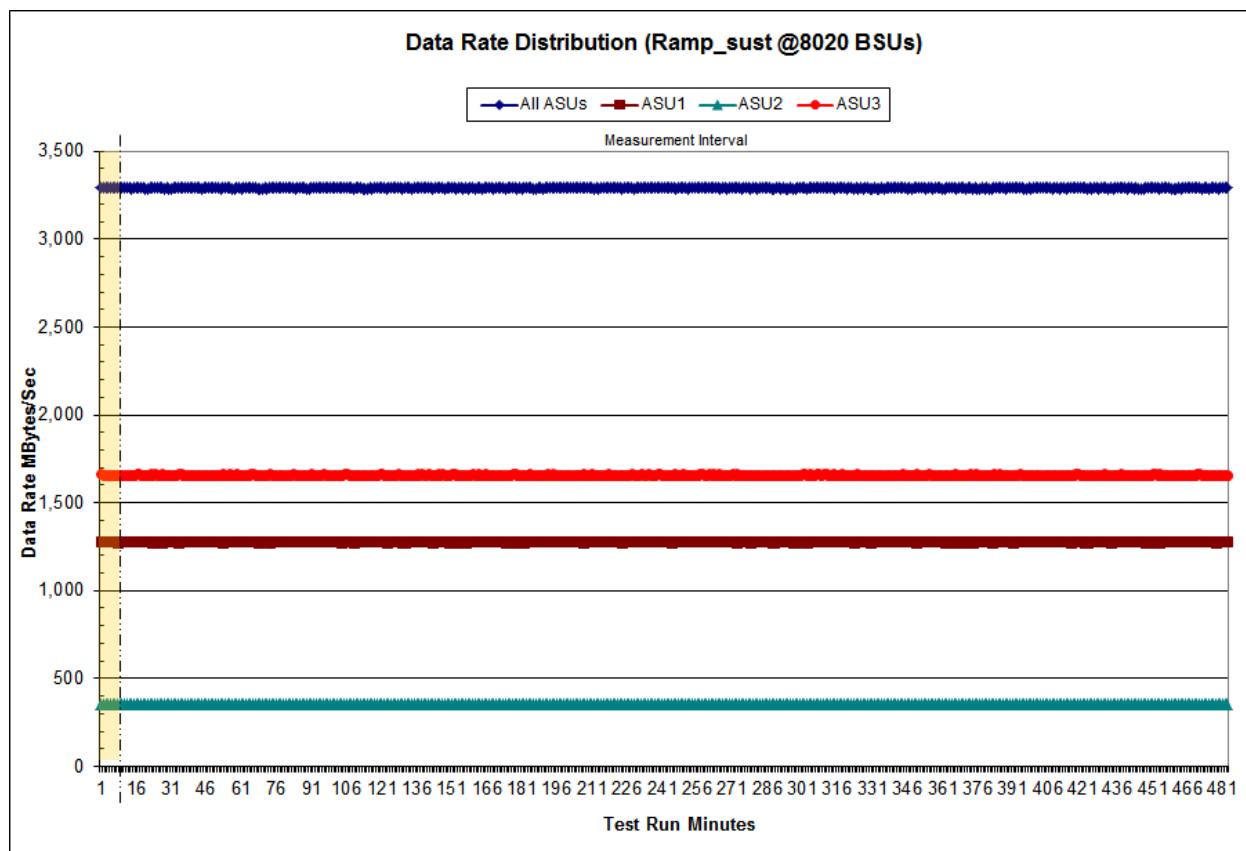


Sustainability – I/O Request Throughput Distribution Data

The Sustainability I/O Request Throughput table of data is not embedded in this document due to its size. The table is available via the following URL:

[Sustainability I/O Request Throughput Table](#)

Sustainability – I/O Request Throughput Distribution Graph

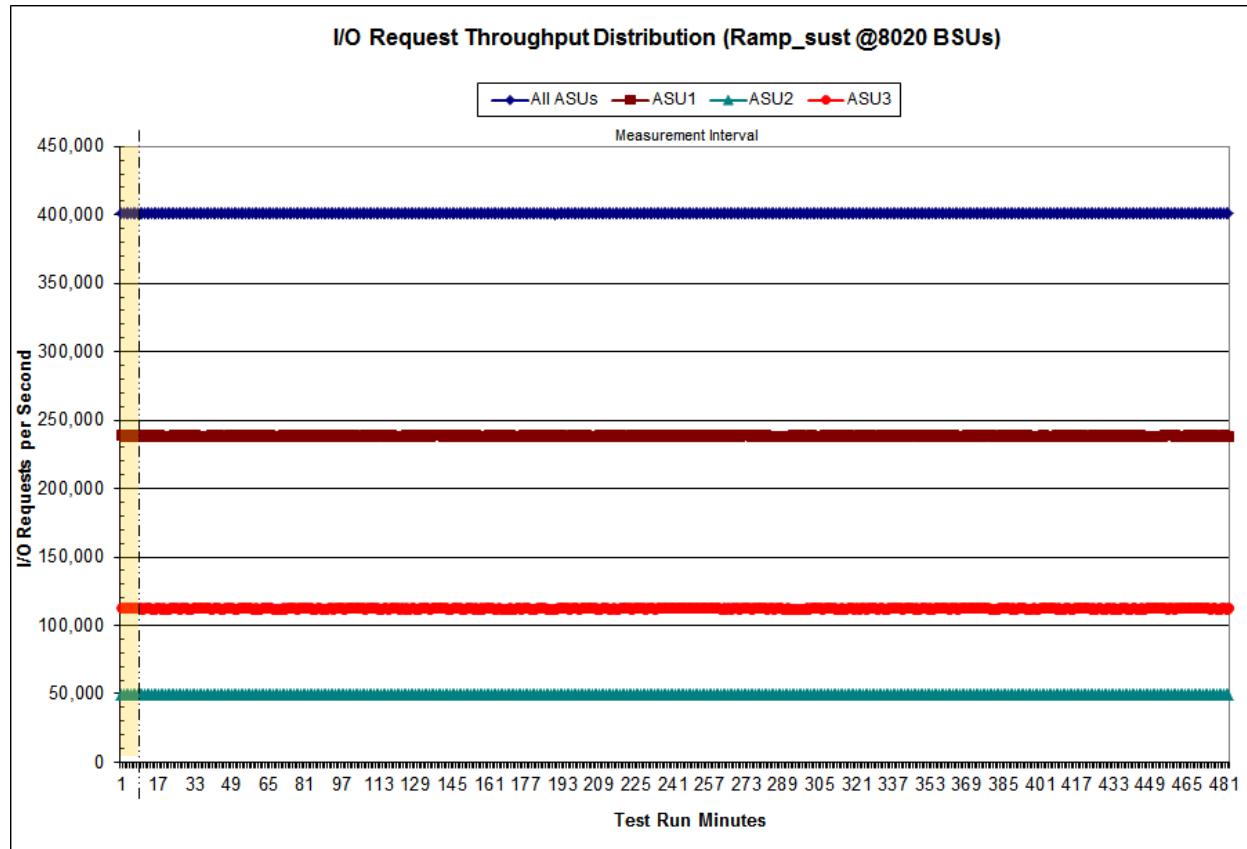


Sustainability – Average Response Time (ms) Distribution Data

The Sustainability Average Response Time table of data is not embedded in this document due to its size. The table is available via the following URL:

[Sustainability Average Response Time Table](#)


Sustainability – Average Response Time (ms) Distribution Graph

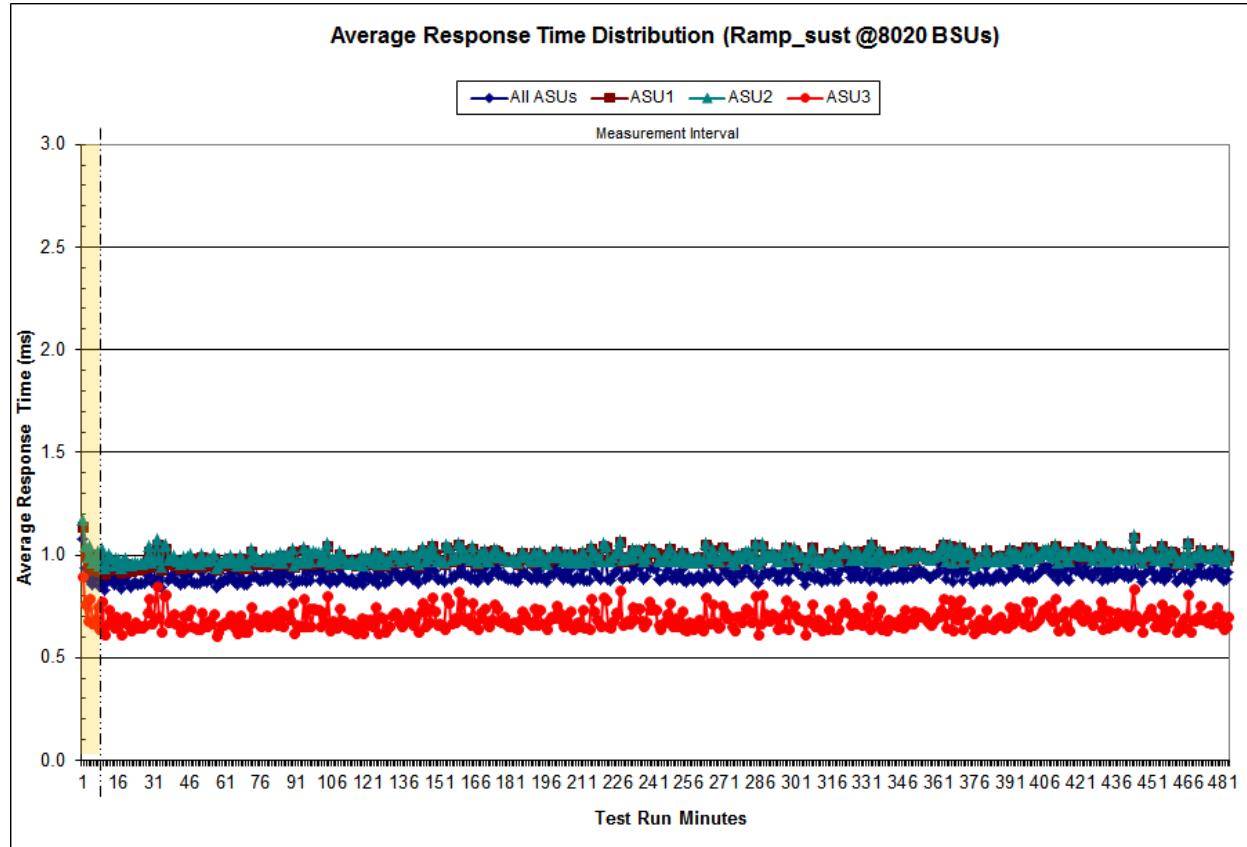

Sustainability – Response Time Frequency Distribution Data

Response Time (ms)	0-0.25	>0.25-0.5	>0.5-0.75	>0.75-1.0	>1.0-1.25	>1.25-1.5	>1.5-1.75	>1.75-2.0
Read	190,180,691	2,582,450,108	691,835,124	157,117,672	84,805,599	61,893,452	51,505,197	45,861,854
Write	430,447,310	4,811,984,707	1,047,223,235	270,920,376	114,207,594	68,545,304	42,602,758	26,878,121
All ASUs	620,628,001	7,394,434,815	1,739,058,359	428,038,048	199,013,193	130,438,756	94,107,955	72,739,975
ASU1	379,052,620	4,326,034,144	978,977,591	238,821,419	118,069,409	80,559,914	61,005,033	49,669,625
ASU2	61,831,319	877,633,446	230,275,961	54,357,141	25,426,166	16,980,983	12,633,822	10,151,003
ASU3	179,744,062	2,190,767,225	529,804,807	134,859,488	55,517,618	32,897,859	20,469,100	12,919,347
Response Time (ms)	>2.0-2.5	>2.5-3.0	>3.0-3.5	>3.5-4.0	>4.0-4.5	>4.5-5.0	>5.0-6.0	>6.0-7.0
Read	82,603,785	75,145,828	61,208,931	53,824,441	49,430,230	45,151,322	78,622,073	63,690,890
Write	31,783,568	19,120,473	13,897,136	10,374,471	8,382,826	6,670,569	10,391,881	8,563,897
All ASUs	114,387,353	94,266,301	75,106,067	64,198,912	57,813,056	51,821,891	89,013,954	72,254,787
ASU1	82,471,074	70,769,938	56,972,856	49,446,173	44,903,068	40,561,526	70,030,768	56,690,878
ASU2	16,694,279	14,352,103	11,472,561	9,757,165	8,859,832	8,013,452	13,881,797	11,316,706
ASU3	15,222,000	9,144,260	6,660,650	4,995,574	4,050,156	3,246,913	5,101,389	4,247,203
Response Time (ms)	>7.0-8.0	>8.0-9.0	>9.0-10.0	>10.0-15.0	>15.0-20.0	>20.0-25.0	>25.0-30.0	>30.0
Read	49,768,054	37,516,327	27,488,811	54,953,097	8,125,813	993,951	205,538	351,481
Write	7,534,096	6,414,314	5,439,446	20,103,588	15,105,099	4,900,604	3,204,727	9,342,885
All ASUs	57,302,150	43,930,641	32,928,257	75,056,685	23,230,912	5,894,555	3,410,265	9,694,366
ASU1	44,575,912	33,858,012	25,069,123	53,814,628	13,056,241	2,883,899	1,537,776	4,294,962
ASU2	8,963,856	6,846,086	5,101,172	11,117,710	2,849,843	650,770	353,078	993,449
ASU3	3,762,382	3,226,543	2,757,962	10,124,347	7,324,828	2,359,886	1,519,411	4,405,955

Sustainability – Response Time Frequency Distribution Graph

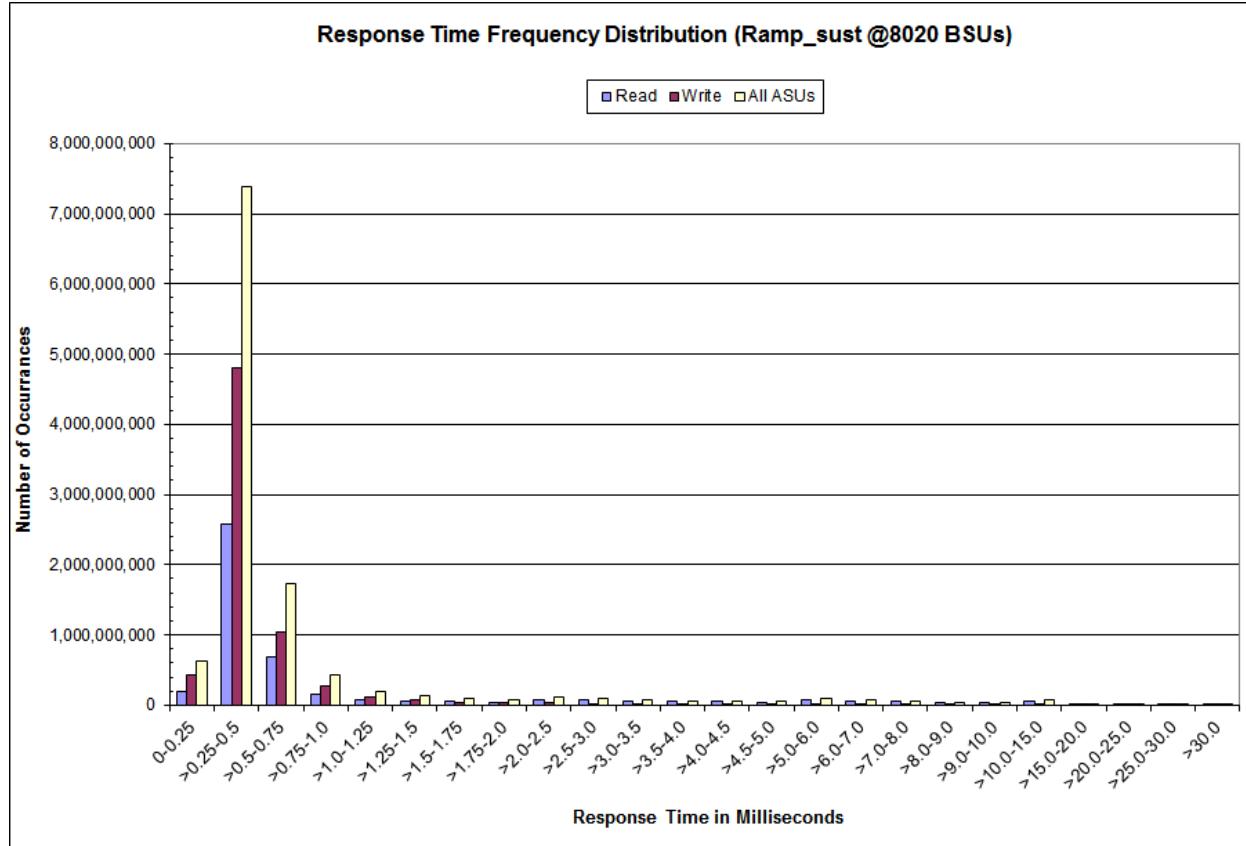

Sustainability – Measured Intensity Multiplier and Coefficient of Variation

Clause 3.4.3

IM – Intensity Multiplier: The ratio of I/Os for each I/O stream relative to the total I/Os for all I/O streams (ASU1-1 – ASU3-1) as required by the benchmark specification.

Clauses 5.1.10 and 5.3.15.2

MIM – Measured Intensity Multiplier: The Measured Intensity Multiplier represents the ratio of measured I/Os for each I/O stream relative to the total I/Os measured for all I/O streams (ASU1-1 – ASU3-1). This value may differ from the corresponding Expected Intensity Multiplier by no more than 5%.

Clause 5.3.15.3

COV – Coefficient of Variation: This measure of variation for the Measured Intensity Multiplier cannot exceed 0.2.

	ASU1-1	ASU1-2	ASU1-3	ASU1-4	ASU2-1	ASU2-2	ASU2-3	ASU3-1
IM	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
MIM	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
COV	0.001	0.000	0.001	0.000	0.002	0.001	0.001	0.000

Primary Metrics Test – IOPS Test Phase

Clause 5.4.4.2

The IOPS Test Phase consists of one Test Run at the 100% load point with a Measurement Interval of ten (10) minutes. The IOPS Test Phase immediately follows the Sustainability Test Phase without any interruption or manual intervention.

The IOPS Test Run generates the SPC-1 IOPSTM primary metric, which is computed as the I/O Request Throughput for the Measurement Interval of the IOPS Test Run.

The Average Response Time is computed for the IOPS Test Run and cannot exceed 30 milliseconds. If the Average Response Time exceeds the 30 millisecond constraint, the measurement is invalid.

Clause 9.4.3.7.3

For the IOPS Test Phase the FDR shall contain:

1. *I/O Request Throughput Distribution (data and graph).*
2. *A Response Time Frequency Distribution.*
3. *An Average Response Time Distribution.*
4. *The human readable Test Run Results File produced by the Workload Generator.*
5. *A listing or screen image of all input parameters supplied to the Workload Generator.*
6. *The total number of I/O Requests completed in the Measurement Interval as well as the number of I/O Requests with a Response Time less than or equal to 30 milliseconds and the number of I/O Requests with a Response Time greater than 30 milliseconds.*

SPC-1 Workload Generator Input Parameters

The SPC-1 Workload Generator input parameters for the Sustainability, IOPS, Response Time Ramp, Repeatability, and Persistence Test Runs are documented in [Appendix E: SPC-1 Workload Generator Input Parameters](#) on Page [83](#).

IOPS Test Results File


A link to the test results file generated from the IOPS Test Run is listed below.

[IOPS Test Results File](#)

IOPS Test Run – I/O Request Throughput Distribution Data

8,020 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up	12:29:24	12:32:25	0-2	0:03:01
Measurement Interval	12:32:25	12:42:25	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	401,007.40	239,030.62	49,351.02	112,625.77
1	401,000.37	238,960.85	49,294.07	112,745.45
2	400,985.37	238,958.32	49,371.05	112,656.00
3	400,848.13	238,852.77	49,296.67	112,698.70
4	400,876.42	238,923.50	49,315.80	112,637.12
5	401,006.00	239,032.00	49,311.48	112,662.52
6	400,919.13	238,956.07	49,344.52	112,618.55
7	401,217.58	239,105.03	49,356.55	112,756.00
8	401,015.68	239,002.65	49,323.42	112,689.62
9	400,966.48	238,961.42	49,344.45	112,660.62
10	401,041.58	239,039.65	49,362.10	112,639.83
11	401,066.20	239,002.38	49,336.17	112,727.65
12	401,097.47	239,151.18	49,320.48	112,625.80
Average	401,005.47	239,002.67	49,331.16	112,671.64


IOPS Test Run – I/O Request Throughput Distribution Graph

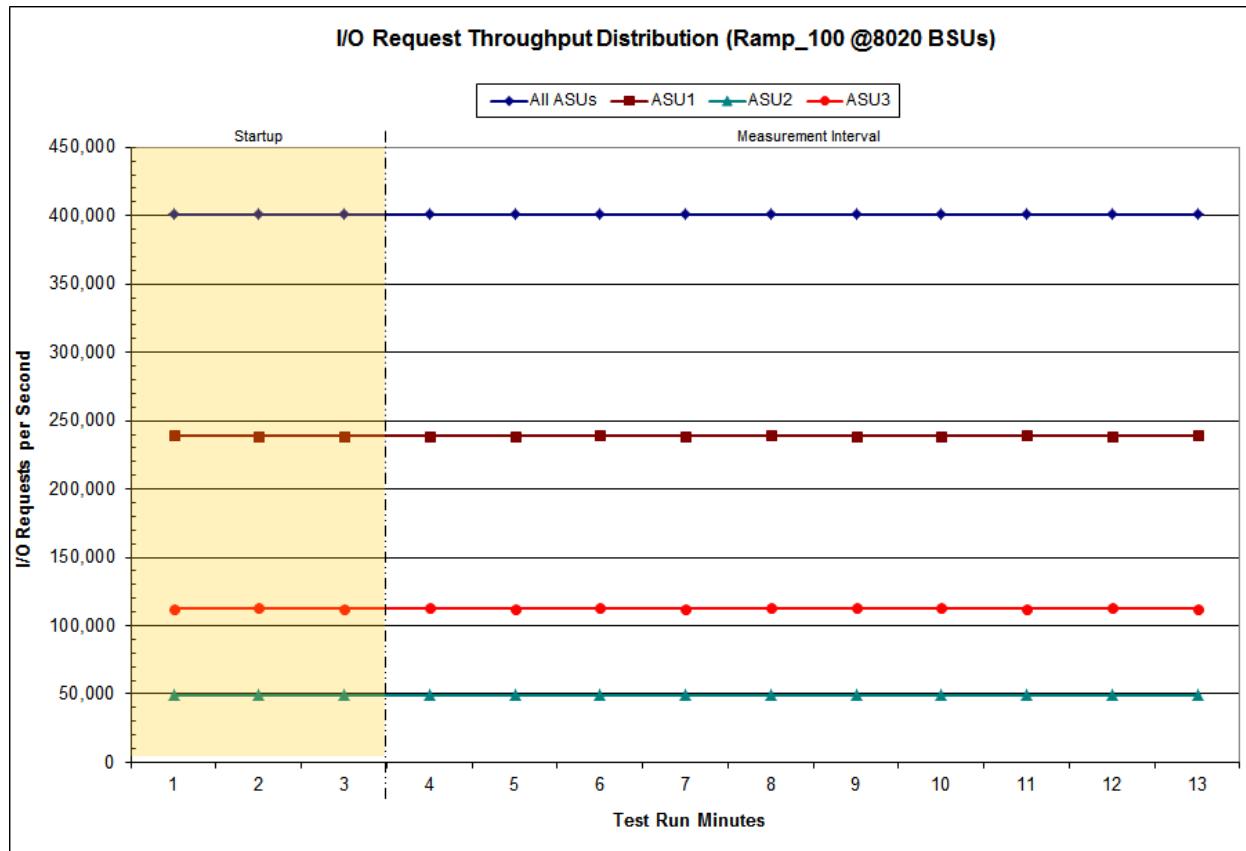

IOPS Test Run – Average Response Time (ms) Distribution Data

8,020 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up	12:29:24	12:32:25	0-2	0:03:01
Measurement Interval	12:32:25	12:42:25	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	0.83	0.88	0.92	0.66
1	0.83	0.90	0.94	0.63
2	0.87	0.93	0.97	0.70
3	0.85	0.91	0.95	0.65
4	0.80	0.88	0.91	0.58
5	0.85	0.92	0.95	0.65
6	0.85	0.91	0.95	0.66
7	0.84	0.91	0.94	0.64
8	0.87	0.93	0.97	0.69
9	0.85	0.92	0.96	0.66
10	0.85	0.92	0.95	0.66
11	0.83	0.90	0.93	0.62
12	0.86	0.93	0.96	0.67
Average	0.84	0.91	0.95	0.65


IOPS Test Run – Average Response Time (ms) Distribution Graph

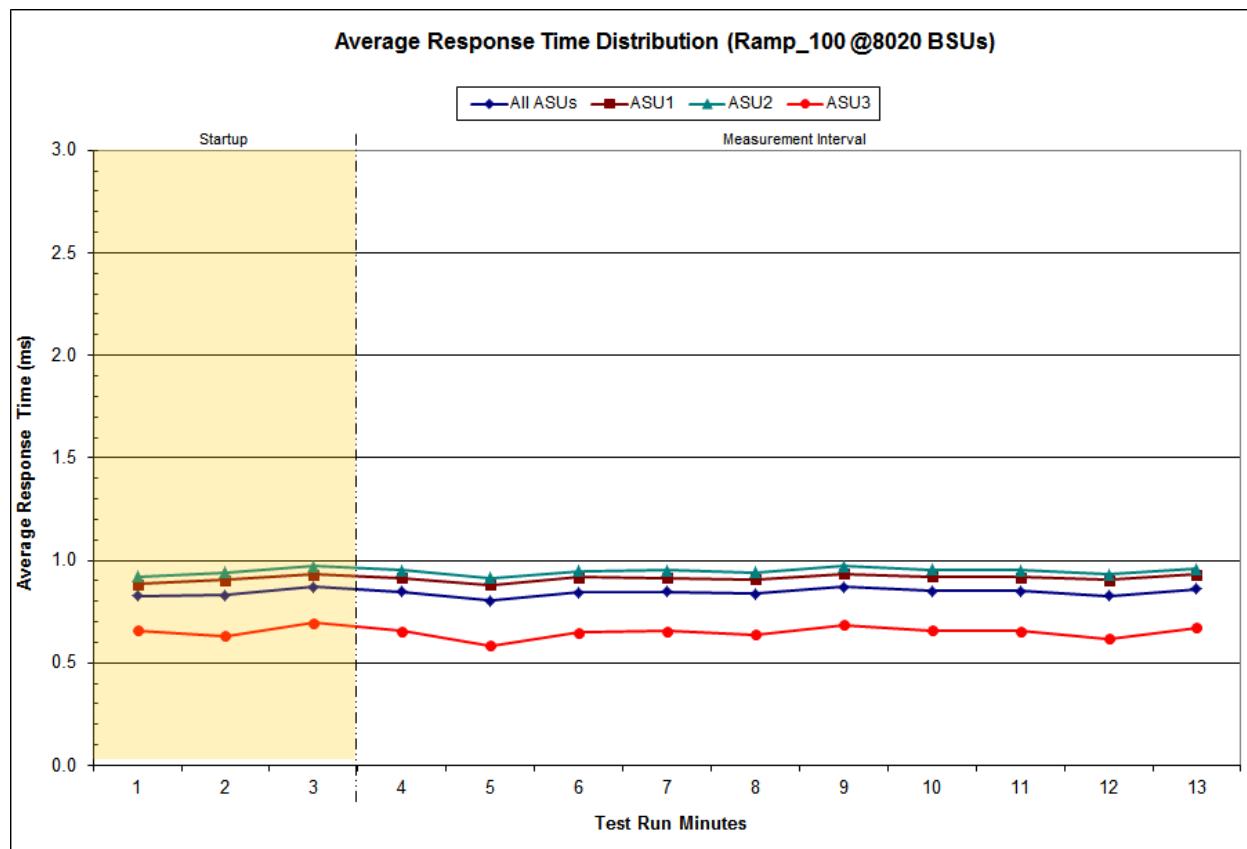

IOPS Test Run –Response Time Frequency Distribution Data

Response Time (ms)	0-0.25	>0.25-0.5	>0.5-0.75	>0.75-1.0	>1.0-1.25	>1.25-1.5	>1.5-1.75	>1.75-2.0
Read	8,226,204	54,337,027	11,794,245	2,630,476	1,517,434	1,144,823	973,873	877,940
Write	12,322,656	102,197,612	18,543,270	4,659,080	2,003,514	1,240,592	769,423	483,690
All ASUs	20,548,860	156,534,639	30,337,515	7,289,556	3,520,948	2,385,415	1,743,296	1,361,630
ASU1	13,660,025	90,768,011	16,771,598	4,035,328	2,089,680	1,472,051	1,131,851	932,093
ASU2	1,763,649	18,922,520	4,117,617	938,790	460,382	319,435	241,413	197,071
ASU3	5,125,186	46,844,108	9,448,300	2,315,438	970,886	593,929	370,032	232,466
Response Time (ms)	>2.0-2.5	>2.5-3.0	>3.0-3.5	>3.5-4.0	>4.0-4.5	>4.5-5.0	>5.0-6.0	>6.0-7.0
Read	1,598,801	1,466,350	1,185,182	1,048,417	964,310	881,415	1,539,277	1,246,138
Write	578,300	355,057	262,645	198,034	161,281	129,000	205,631	173,973
All ASUs	2,177,101	1,821,407	1,447,827	1,246,451	1,125,591	1,010,415	1,744,908	1,420,111
ASU1	1,568,953	1,362,818	1,093,642	954,036	867,848	785,245	1,362,383	1,102,958
ASU2	330,969	289,064	228,650	197,057	179,346	162,680	281,340	230,595
ASU3	277,179	169,525	125,535	95,358	78,397	62,490	101,185	86,558
Response Time (ms)	>7.0-8.0	>8.0-9.0	>9.0-10.0	>10.0-15.0	>15.0-20.0	>20.0-25.0	>25.0-30.0	>30.0
Read	971,695	729,212	531,106	1,048,821	150,042	17,638	3,357	3,689
Write	154,716	131,528	110,737	413,539	309,236	96,964	62,392	152,638
All ASUs	1,126,411	860,740	641,843	1,462,360	459,278	114,602	65,749	156,327
ASU1	866,341	655,969	482,861	1,031,812	253,075	55,179	29,313	68,330
ASU2	182,495	138,527	102,911	222,692	56,055	12,554	6,951	15,892
ASU3	77,575	66,244	56,071	207,856	150,148	46,869	29,485	72,105

IOPS Test Run –Response Time Frequency Distribution Graph

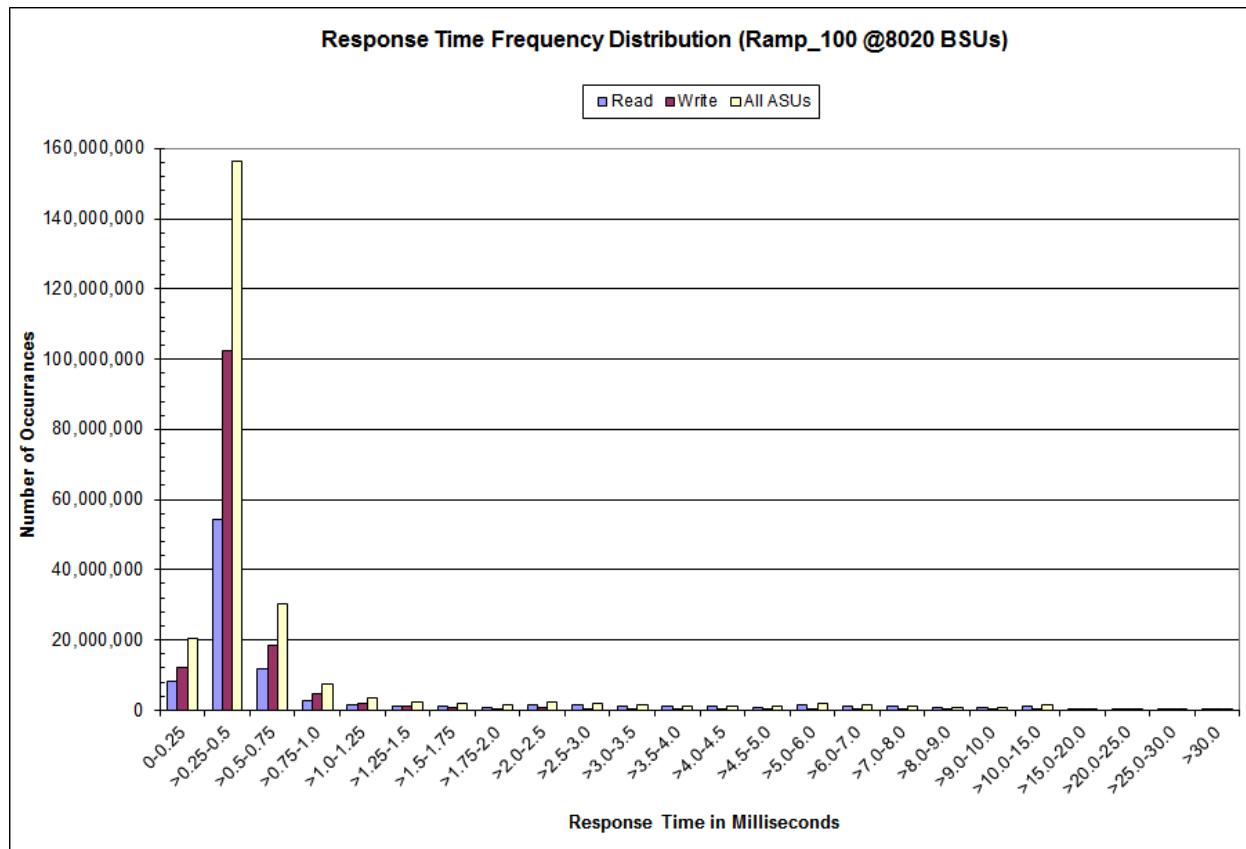

IOPS Test Run – I/O Request Information

I/O Requests Completed in the Measurement Interval
240,602.980
I/O Requests Completed with Response Time = or < 30 ms
240,446,653
I/O Requests Completed with Response Time > 30 ms
156.327

IOPS Test Run – Measured Intensity Multiplier and Coefficient of Variation

Clause 3.4.3

IM – Intensity Multiplier: The ratio of I/Os for each I/O stream relative to the total I/Os for all I/O streams (ASU1-1 – ASU3-1) as required by the benchmark specification.

Clauses 5.1.10 and 5.3.15.2

MIM – Measured Intensity Multiplier: The Measured Intensity Multiplier represents the ratio of measured I/Os for each I/O stream relative to the total I/Os measured for all I/O streams (ASU1-1 – ASU3-1). This value may differ from the corresponding Expected Intensity Multiplier by no more than 5%.

Clause 5.3.15.3

COV – Coefficient of Variation: This measure of variation for the Measured Intensity Multiplier cannot exceed 0.2.

	ASU1-1	ASU1-2	ASU1-3	ASU1-4	ASU2-1	ASU2-2	ASU2-3	ASU3-1
IM	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
MIM	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
COV	0.001	0.000	0.001	0.001	0.002	0.000	0.001	0.000

Primary Metrics Test – Response Time Ramp Test Phase

Clause 5.4.4.3

The Response Time Ramp Test Phase consists of five Test Runs, one each at 95%, 90%, 80%, 50%, and 10% of the load point (100%) used to generate the SPC-1 IOPSTM primary metric. Each of the five Test Runs has a Measurement Interval of ten (10) minutes. The Response Time Ramp Test Phase immediately follows the IOPS Test Phase without any interruption or manual intervention.

The five Response Time Ramp Test Runs, in conjunction with the IOPS Test Run (100%), demonstrate the relationship between Average Response Time and I/O Request Throughput for the Tested Storage Configuration (TSC) as illustrated in the response time/throughput curve on page 16.

In addition, the Average Response Time measured during the 10% Test Run is the value for the SPC-1 LRT™ metric. That value represents the Average Response Time of a lightly loaded TSC.

Clause 9.4.3.7.4

The following content shall appear in the FDR for the Response Time Ramp Phase:

1. *A Response Time Ramp Distribution.*
2. *The human readable Test Run Results File produced by the Workload Generator for each Test Run within the Response Time Ramp Test Phase.*
3. *For the 10% Load Level Test Run (SPC-1 LRT™ metric) an Average Response Time Distribution.*
4. *A listing or screen image of all input parameters supplied to the Workload Generator.*

SPC-1 Workload Generator Input Parameters

The SPC-1 Workload Generator input parameters for the Sustainability, IOPS, Response Time Ramp, Repeatability, and Persistence Test Runs are documented in [Appendix E: SPC-1 Workload Generator Input Parameters](#) on Page [83](#).

Response Time Ramp Test Results File

A link to each test result file generated from each Response Time Ramp Test Run listed below.

[95% Load Level](#)

[90% Load Level](#)

[80% Load Level](#)

[50% Load Level](#)

[10% Load Level](#)

Response Time Ramp Distribution (IOPS) Data


The five Test Runs that comprise the Response Time Ramp Phase are executed at 95%, 90%, 80%, 50%, and 10% of the Business Scaling Unit (BSU) load level used to produce the SPC-1 IOPSTM primary metric. The 100% BSU load level is included in the following Response Time Ramp data table and graph for completeness.

100% Load Level: 8,020 BSUs				95% Load Level: 7,619 BSUs					
Start-Up/Ramp-Up	Start	Stop	Interval	Duration	Start-Up/Ramp-Up	Start	Stop	Interval	Duration
Measurement Interval	12:29:24	12:32:25	0-3	0:03:01	Measurement Interval	12:43:10	12:46:11	0-3	0:03:01
(60 second intervals)	All ASUs	ASU-1	ASU-2	ASU-3	(60 second intervals)	All ASUs	ASU-1	ASU-2	ASU-3
0	401,007.40	239,030.62	49,351.02	112,625.77	0	381,059.05	227,140.97	46,883.75	107,034.33
1	401,000.37	238,960.85	49,294.07	112,745.45	1	380,922.37	227,002.40	46,849.40	107,070.57
2	400,985.37	238,958.32	49,371.05	112,656.00	2	381,055.90	227,077.68	46,892.75	107,085.47
3	400,848.13	238,852.77	49,296.67	112,698.70	3	381,045.53	227,117.17	46,859.40	107,068.97
4	400,876.42	238,923.50	49,315.80	112,637.12	4	381,011.68	227,043.87	46,879.43	107,088.38
5	401,006.00	239,032.00	49,311.48	112,662.52	5	380,848.72	226,981.75	46,863.30	107,003.67
6	400,919.13	238,956.07	49,344.52	112,618.55	6	380,953.13	227,074.47	46,834.25	107,044.42
7	401,217.58	239,105.03	49,356.55	112,756.00	7	381,006.83	227,072.00	46,852.30	107,082.53
8	401,015.68	239,002.65	49,323.42	112,689.62	8	380,812.68	226,954.12	46,858.67	106,999.90
9	400,966.48	238,961.42	49,344.45	112,660.62	9	380,905.63	226,979.67	46,860.67	107,065.30
10	401,041.58	239,039.65	49,362.10	112,639.83	10	381,055.05	227,089.72	46,877.08	107,088.25
11	401,066.20	239,002.38	49,336.17	112,727.65	11	381,020.58	227,052.65	46,912.37	107,055.57
12	401,097.47	239,151.18	49,320.48	112,625.80	12	381,131.52	227,164.35	46,837.00	107,130.17
Average	401,005.47	239,002.67	49,331.16	112,671.64	Average	380,979.14	227,052.98	46,863.45	107,062.72
90% Load Level: 7,218 BSUs				80% Load Level: 6,416 BSUs					
Start-Up/Ramp-Up	Start	Stop	Interval	Duration	Start-Up/Ramp-Up	Start	Stop	Interval	Duration
Measurement Interval	12:56:54	12:59:55	0-3	0:03:01	Measurement Interval	13:10:34	13:13:35	0-3	0:03:01
(60 second intervals)	All ASUs	ASU-1	ASU-2	ASU-3	(60 second intervals)	All ASUs	ASU-1	ASU-2	ASU-3
0	361,190.58	215,205.57	44,459.10	101,525.92	0	320,840.10	191,246.87	39,446.08	90,147.15
1	361,014.25	215,168.90	44,393.33	101,452.02	1	320,802.07	191,195.55	39,456.67	90,149.85
2	360,839.15	215,057.37	44,395.10	101,386.68	2	320,807.35	191,226.80	39,446.52	90,134.03
3	361,017.67	215,111.72	44,393.02	101,512.93	3	320,765.78	191,151.43	39,481.28	90,133.07
4	360,904.77	215,035.62	44,399.17	101,469.98	4	320,747.67	191,191.42	39,476.68	90,079.57
5	360,991.87	215,085.55	44,413.72	101,492.60	5	320,728.45	191,177.33	39,421.18	90,129.93
6	360,832.15	215,071.85	44,412.22	101,348.08	6	320,905.80	191,281.23	39,488.45	90,136.12
7	360,962.05	215,133.78	44,379.35	101,448.92	7	320,879.53	191,234.68	39,472.70	90,172.15
8	360,730.70	215,035.35	44,356.42	101,338.93	8	320,821.92	191,230.08	39,453.93	90,137.90
9	360,949.30	215,172.30	44,364.35	101,412.65	9	320,750.25	191,175.72	39,458.02	90,116.52
10	360,942.78	215,138.95	44,381.05	101,422.78	10	320,880.70	191,241.07	39,480.00	90,159.63
11	360,940.88	215,170.10	44,406.37	101,364.42	11	320,761.77	191,139.47	39,480.03	90,142.27
12	360,913.93	215,115.83	44,378.28	101,419.82	12	320,905.25	191,197.60	39,488.43	90,219.22
Average	360,918.61	215,107.11	44,388.39	101,423.11	Average	320,814.71	191,202.00	39,470.07	90,142.64

Response Time Ramp Distribution (IOPS) Data (*continued*)

50% Load Level: 4,010 BSUs	Start	Stop	Interval	Duration	10% Load Level: 802 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up Measurement Interval	13:24:04	13:27:05	0-3	0:03:01	Start-Up/Ramp-Up Measurement Interval	13:37:20	13:40:21	0-3	0:03:01
(60 second intervals)	13:27:05	13:37:05	3-12	0:10:00	(60 second intervals)	13:40:21	13:50:21	3-12	0:10:00
0	200,568.08	119,550.18	24,670.68	56,347.22	0	40,113.38	23,910.05	4,946.15	11,257.18
1	200,628.42	119,586.35	24,658.72	56,383.35	1	40,144.02	23,951.02	4,932.45	11,260.55
2	200,455.02	119,455.18	24,682.85	56,316.98	2	40,086.13	23,886.57	4,930.73	11,268.83
3	200,485.87	119,487.43	24,660.95	56,337.48	3	40,120.87	23,906.42	4,939.03	11,275.42
4	200,415.70	119,451.65	24,621.68	56,342.37	4	40,095.23	23,891.00	4,937.82	11,266.42
5	200,663.98	119,563.82	24,704.05	56,396.12	5	40,078.42	23,888.28	4,928.93	11,261.20
6	200,440.08	119,444.07	24,669.32	56,326.70	6	40,094.55	23,880.57	4,940.55	11,273.43
7	200,565.43	119,535.78	24,659.35	56,370.30	7	40,081.83	23,892.62	4,921.53	11,267.68
8	200,521.00	119,562.32	24,643.82	56,314.87	8	40,098.33	23,900.57	4,932.10	11,265.67
9	200,495.85	119,501.97	24,642.02	56,351.87	9	40,149.42	23,922.47	4,950.60	11,276.35
10	200,573.27	119,508.82	24,688.58	56,375.87	10	40,064.75	23,867.48	4,925.30	11,271.97
11	200,546.62	119,536.37	24,635.95	56,374.30	11	40,125.23	23,901.93	4,958.43	11,264.87
12	200,530.62	119,524.10	24,670.05	56,336.47	12	40,135.60	23,925.97	4,932.05	11,277.58
Average	200,523.84	119,511.63	24,659.58	56,352.63	Average	40,104.42	23,897.73	4,936.64	11,270.06


Response Time Ramp Distribution (IOPS) Graph

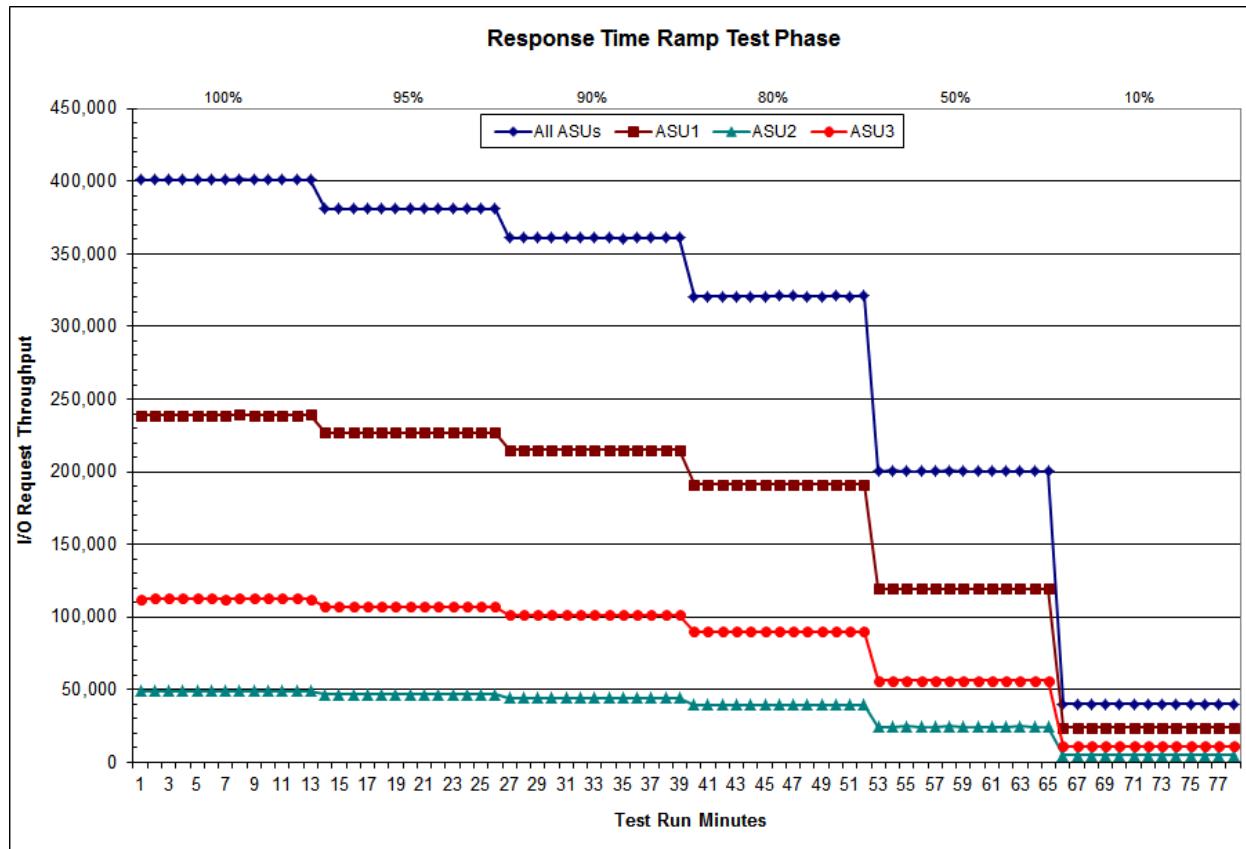

SPC-1 LRT™ Average Response Time (ms) Distribution Data

802 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up	13:37:20	13:40:21	0-2	0:03:01
Measurement Interval	13:40:21	13:50:21	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	0.38	0.36	0.38	0.40
1	0.39	0.38	0.40	0.40
2	0.38	0.38	0.40	0.39
3	0.39	0.38	0.40	0.39
4	0.38	0.38	0.40	0.39
5	0.39	0.38	0.40	0.40
6	0.38	0.38	0.40	0.39
7	0.40	0.39	0.41	0.41
8	0.38	0.38	0.40	0.39
9	0.39	0.38	0.40	0.40
10	0.39	0.38	0.41	0.40
11	0.39	0.38	0.40	0.40
12	0.39	0.38	0.40	0.40
Average	0.39	0.38	0.40	0.40

SPC-1 LRT™ Average Response Time (ms) Distribution Graph

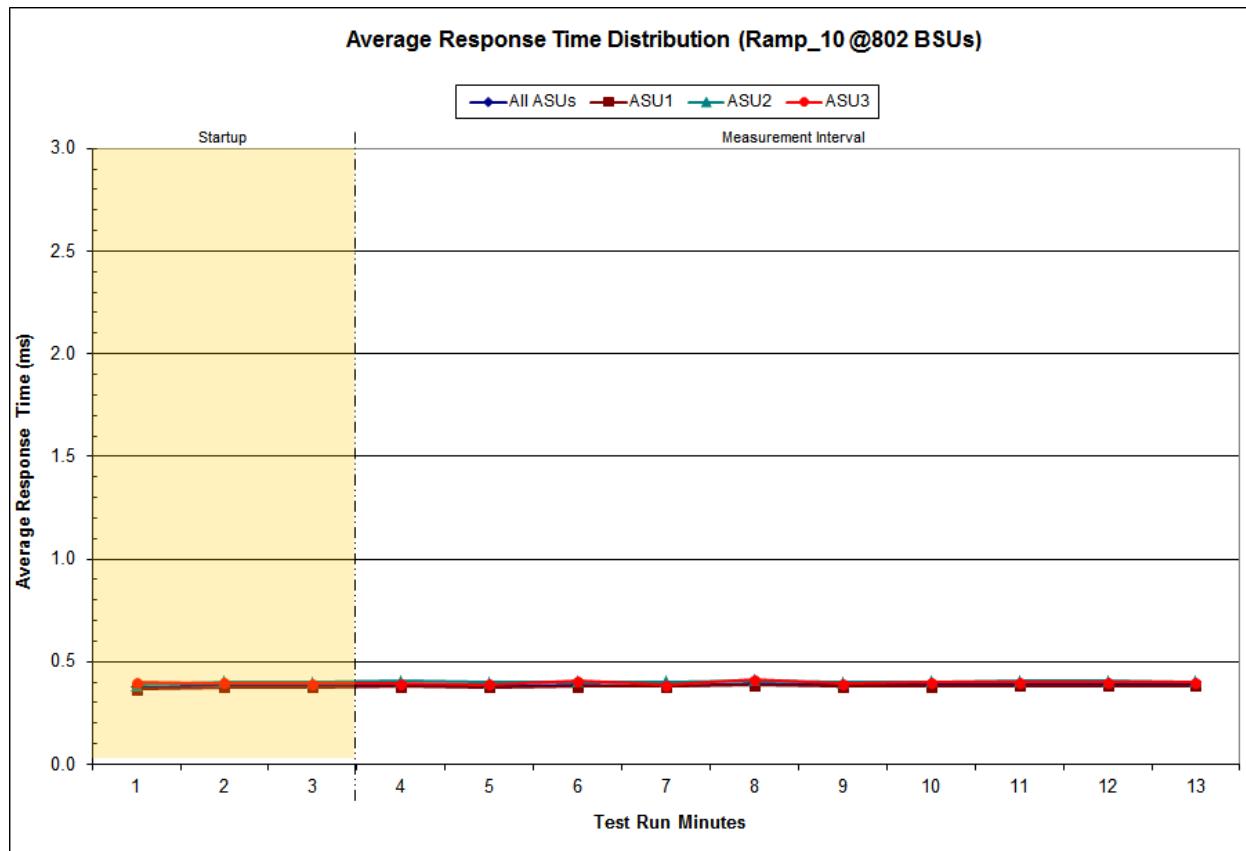

SPC-1 LRT™ (10%) – Measured Intensity Multiplier and Coefficient of Variation

Clause 3.4.3

IM – Intensity Multiplier: The ratio of I/Os for each I/O stream relative to the total I/Os for all I/O streams (ASU1-1 – ASU3-1) as required by the benchmark specification.

Clauses 5.1.10 and 5.3.15.2

MIM – Measured Intensity Multiplier: The Measured Intensity Multiplier represents the ratio of measured I/Os for each I/O stream relative to the total I/Os measured for all I/O streams (ASU1-1 – ASU3-1). This value may differ from the corresponding Expected Intensity Multiplier by no more than 5%.

Clause 5.3.15.3

COV – Coefficient of Variation: This measure of variation for the Measured Intensity Multiplier cannot exceed 0.2.

	ASU1-1	ASU1-2	ASU1-3	ASU1-4	ASU2-1	ASU2-2	ASU2-3	ASU3-1
IM	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
MIM	0.0350	0.2810	0.0700	0.2099	0.0180	0.0700	0.0351	0.2810
COV	0.003	0.001	0.002	0.001	0.005	0.002	0.003	0.001

Repeatability Test

Clause 5.4.5

The Repeatability Test demonstrates the repeatability and reproducibility of the SPC-1 IOPS™ primary metric and the SPC-1 LRT™ metric generated in earlier Test Runs.

There are two identical Repeatability Test Phases. Each Test Phase contains two Test Runs. Each of the Test Runs will have a Measurement Interval of no less than ten (10) minutes. The two Test Runs in each Test Phase will be executed without interruption or any type of manual intervention.

The first Test Run in each Test Phase is executed at the 10% load point. The Average Response Time from each of the Test Runs is compared to the SPC-1 LRT™ metric. Each Average Response Time value must be less than the SPC-1 LRT™ metric plus 5% or less than the SPC-1 LRT™ metric plus one (1) millisecond (ms).

The second Test Run in each Test Phase is executed at the 100% load point. The I/O Request Throughput from the Test Runs is compared to the SPC-1 IOPS™ primary metric. Each I/O Request Throughput value must be greater than the SPC-1 IOPS™ primary metric minus 5%. In addition, the Average Response Time for each Test Run cannot exceed 30 milliseconds.

If any of the above constraints are not met, the benchmark measurement is invalid.

Clause 9.4.3.7.5

The following content shall appear in the FDR for each Test Run in the two Repeatability Test Phases:

1. A table containing the results of the Repeatability Test.
2. An I/O Request Throughput Distribution graph and table.
3. An Average Response Time Distribution graph and table.
4. The human readable Test Run Results File produced by the Workload Generator.
5. A listing or screen image of all input parameters supplied to the Workload Generator.

SPC-1 Workload Generator Input Parameters

The SPC-1 Workload Generator input parameters for the Sustainability, IOPS, Response Time Ramp, Repeatability, and Persistence Test Runs are documented in [Appendix E: SPC-1 Workload Generator Input Parameters](#) on Page [83](#).

Repeatability Test Results File

The values for the SPC-1 IOPS™, SPC-1 LRT™, and the Repeatability Test measurements are listed in the tables below.

	SPC-1 IOPS™
Primary Metrics	401,005.47
Repeatability Test Phase 1	401,044.25
Repeatability Test Phase 2	400,995.67

The SPC-1 IOPS™ values in the above table were generated using 100% of the specified Business Scaling Unit (BSU) load level. Each of the Repeatability Test Phase values for SPC-1 IOPS™ must greater than 95% of the reported SPC-1 IOPS™ Primary Metric.

	SPC-1 LRT™
Primary Metrics	0.39
Repeatability Test Phase 1	0.39
Repeatability Test Phase 2	0.39

The average response time values in the SPC-1 LRT™ column were generated using 10% of the specified Business Scaling Unit (BSU) load level. Each of the Repeatability Test Phase values for SPC-1 LRT™ must be less than 105% of the reported SPC-1 LRT™ Primary Metric or less than the reported SPC-1 LRT™ Primary Metric plus one (1) millisecond (ms).

A link to the test result file generated from each Repeatability Test Run is listed below.

[Repeatability Test Phase 1, Test Run 1 \(LRT\)](#)

[Repeatability Test Phase 1, Test Run 2 \(IOPS\)](#)


[Repeatability Test Phase 2, Test Run 1 \(LRT\)](#)

[Repeatability Test Phase 2, Test Run 2 \(IOPS\)](#)

Repeatability 1 LRT – I/O Request Throughput Distribution Data

802 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up	13:50:43	13:53:43	0-2	0:03:00
Measurement Interval	13:53:43	14:03:43	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	40,139.07	23,927.60	4,936.72	11,274.75
1	40,080.18	23,900.35	4,928.48	11,251.35
2	40,071.87	23,841.85	4,942.08	11,287.93
3	40,117.60	23,914.92	4,940.60	11,262.08
4	40,127.75	23,905.70	4,944.80	11,277.25
5	40,051.98	23,872.57	4,937.77	11,241.65
6	40,131.18	23,913.27	4,933.50	11,284.42
7	40,088.07	23,898.22	4,936.15	11,253.70
8	40,105.90	23,909.78	4,935.60	11,260.52
9	40,088.68	23,877.83	4,946.58	11,264.27
10	40,083.45	23,872.48	4,931.73	11,279.23
11	40,089.52	23,892.98	4,935.17	11,261.37
12	40,118.82	23,908.37	4,950.58	11,259.87
Average	40,100.30	23,896.61	4,939.25	11,264.44


Repeatability 1 LRT – I/O Request Throughput Distribution Graph

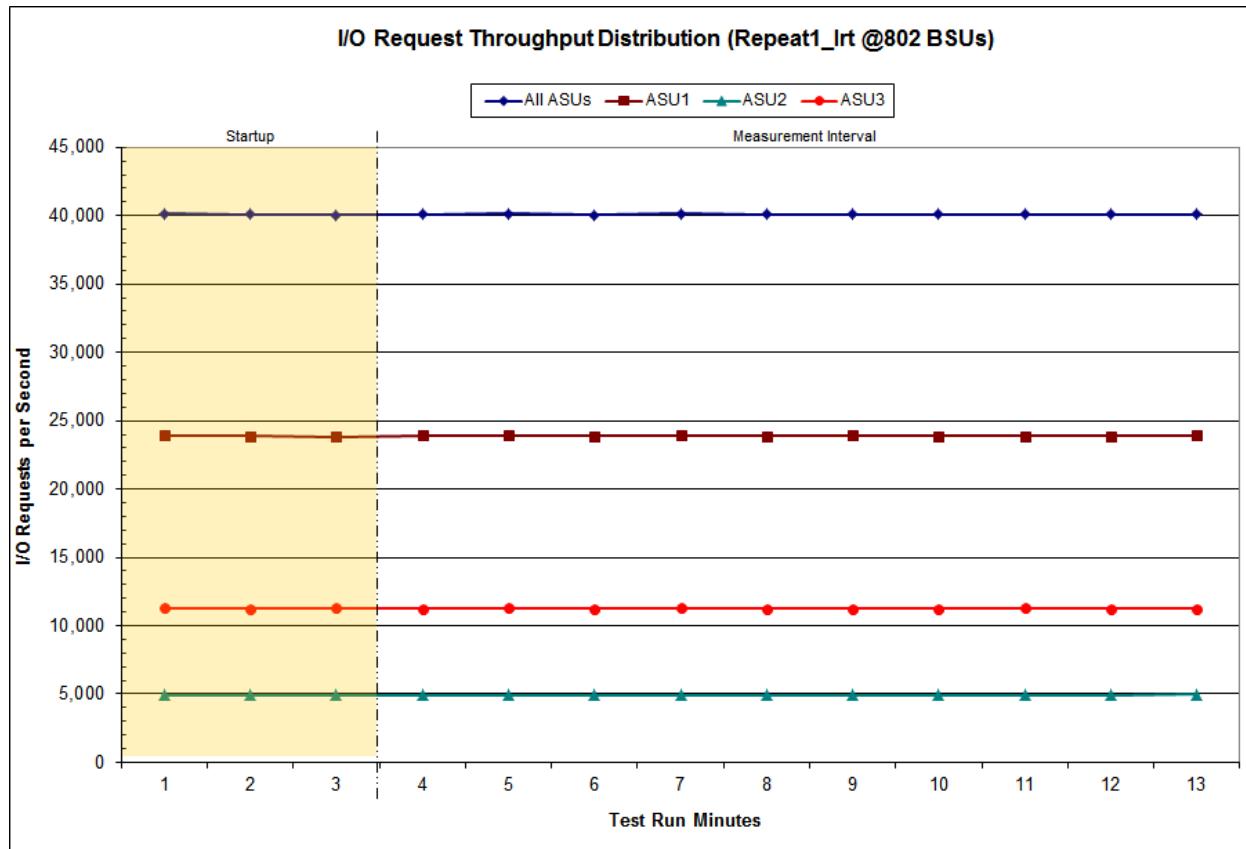

Repeatability 1 LRT –Average Response Time (ms) Distribution Data

802 BSUs	Start	Stop	Interval	Duration
<i>Start-Up/Ramp-Up</i>	13:50:43	13:53:43	0-2	0:03:00
<i>Measurement Interval</i>	13:53:43	14:03:43	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	0.37	0.36	0.38	0.39
1	0.38	0.37	0.40	0.39
2	0.38	0.38	0.40	0.39
3	0.39	0.38	0.41	0.41
4	0.38	0.37	0.40	0.39
5	0.39	0.38	0.40	0.40
6	0.39	0.38	0.40	0.39
7	0.38	0.38	0.40	0.38
8	0.39	0.38	0.41	0.40
9	0.39	0.38	0.41	0.39
10	0.39	0.38	0.40	0.40
11	0.38	0.37	0.40	0.38
12	0.38	0.38	0.40	0.39
Average	0.39	0.38	0.40	0.39


Repeatability 1 LRT –Average Response Time (ms) Distribution Graph

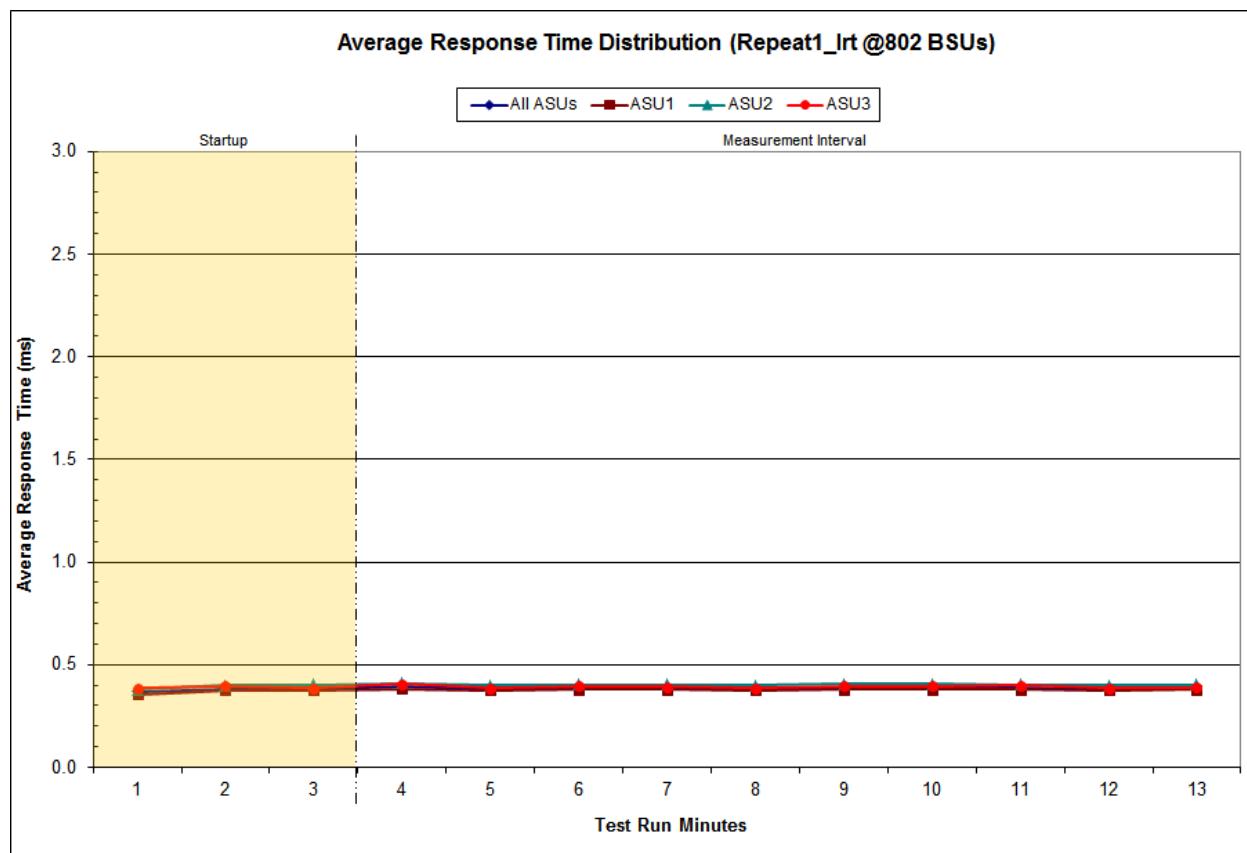

Repeatability 1 IOPS – I/O Request Throughput Distribution Data

8,020 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up	14:04:32	14:07:33	0-2	0:03:01
Measurement Interval	14:07:33	14:17:33	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	401,153.42	239,084.47	49,369.80	112,699.15
1	401,016.73	239,003.33	49,346.52	112,666.88
2	400,920.15	238,916.38	49,321.93	112,681.83
3	401,137.53	239,052.35	49,340.75	112,744.43
4	400,969.32	238,928.30	49,322.98	112,718.03
5	401,092.73	239,095.67	49,325.42	112,671.65
6	400,941.03	238,927.15	49,295.27	112,718.62
7	401,043.58	239,063.78	49,294.70	112,685.10
8	401,094.00	239,047.55	49,327.53	112,718.92
9	400,943.95	238,991.07	49,326.17	112,626.72
10	401,069.65	238,960.70	49,380.92	112,728.03
11	401,130.12	239,030.97	49,363.13	112,736.02
12	401,020.62	238,970.22	49,336.22	112,714.18
Average	401,044.25	239,006.78	49,331.31	112,706.17


Repeatability 1 IOPS – I/O Request Throughput Distribution Graph

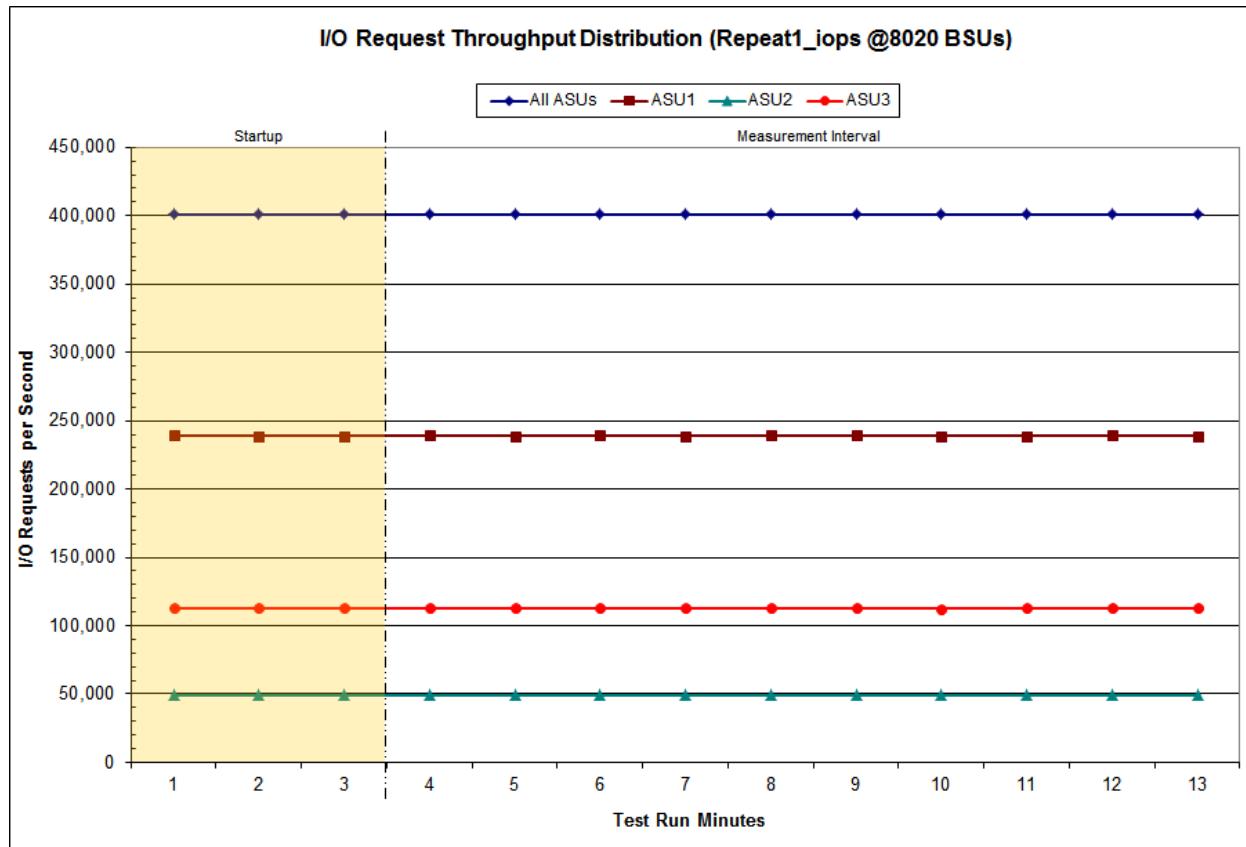

Repeatability 1 IOPS –Average Response Time (ms) Distribution Data

8,020 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up	14:04:32	14:07:33	0-2	0:03:01
Measurement Interval	14:07:33	14:17:33	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	0.84	0.89	0.93	0.68
1	0.87	0.93	0.98	0.70
2	0.84	0.91	0.95	0.66
3	0.83	0.90	0.94	0.64
4	0.86	0.92	0.96	0.68
5	0.89	0.95	0.99	0.72
6	0.83	0.90	0.94	0.62
7	0.89	0.95	0.99	0.72
8	0.85	0.92	0.96	0.65
9	0.83	0.91	0.94	0.63
10	0.88	0.95	0.98	0.71
11	0.84	0.91	0.94	0.63
12	0.85	0.92	0.95	0.66
Average	0.86	0.92	0.96	0.67


Repeatability 1 IOPS –Average Response Time (ms) Distribution Graph

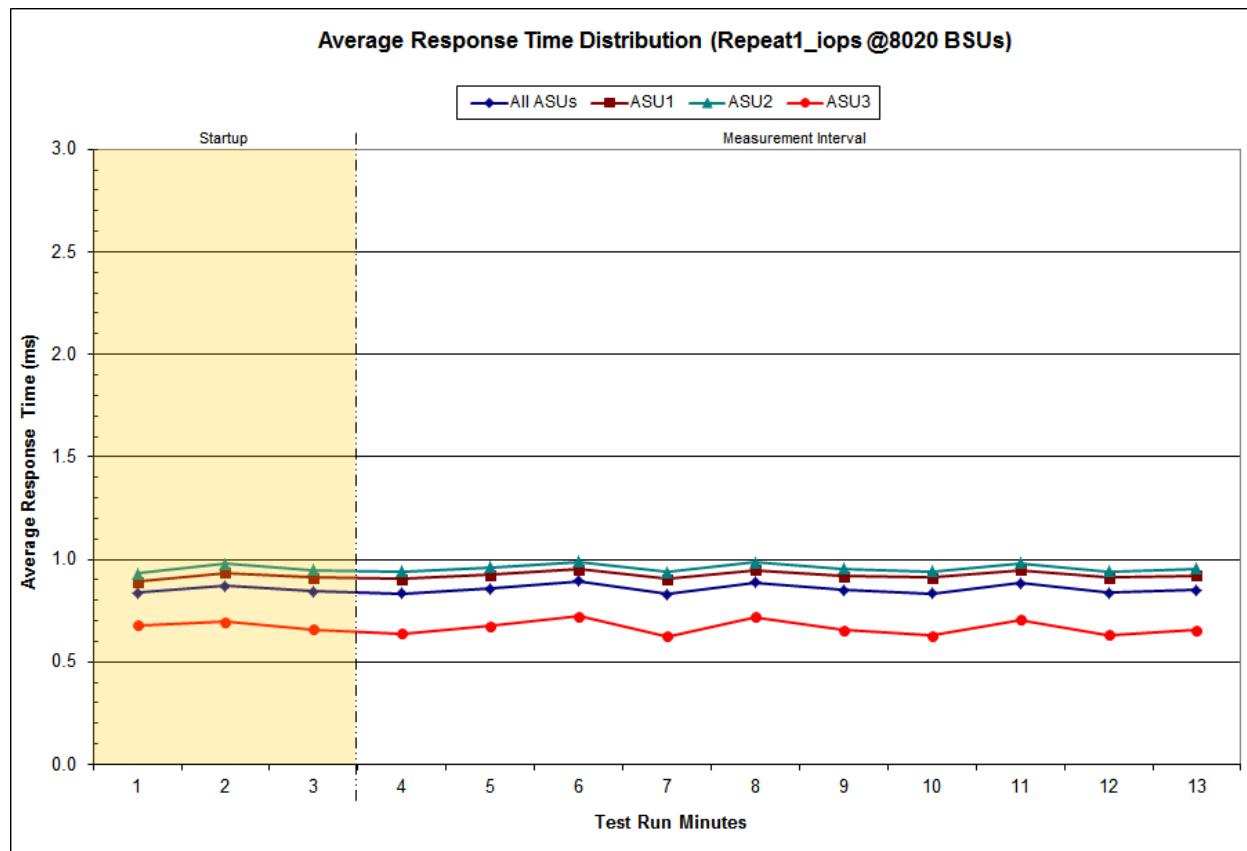

Repeatability 2 LRT – I/O Request Throughput Distribution Data

802 BSUs	Start	Stop	Interval	Duration
<i>Start-Up/Ramp-Up</i>	14:17:54	14:20:54	0-2	0:03:00
<i>Measurement Interval</i>	14:20:54	14:30:54	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	40,085.42	23,888.17	4,922.82	11,274.43
1	40,088.42	23,900.15	4,935.08	11,253.18
2	40,085.72	23,905.12	4,926.77	11,253.83
3	40,098.28	23,898.12	4,931.15	11,269.02
4	40,102.93	23,905.42	4,928.52	11,269.00
5	40,101.60	23,899.55	4,947.32	11,254.73
6	40,089.57	23,890.00	4,948.17	11,251.40
7	40,078.92	23,894.12	4,929.20	11,255.60
8	40,102.20	23,900.05	4,928.55	11,273.60
9	40,104.90	23,890.20	4,939.67	11,275.03
10	40,084.27	23,904.40	4,931.45	11,248.42
11	40,116.57	23,903.97	4,938.88	11,273.72
12	40,098.40	23,906.47	4,933.08	11,258.85
Average	40,097.76	23,899.23	4,935.60	11,262.94


Repeatability 2 LRT – I/O Request Throughput Distribution Graph

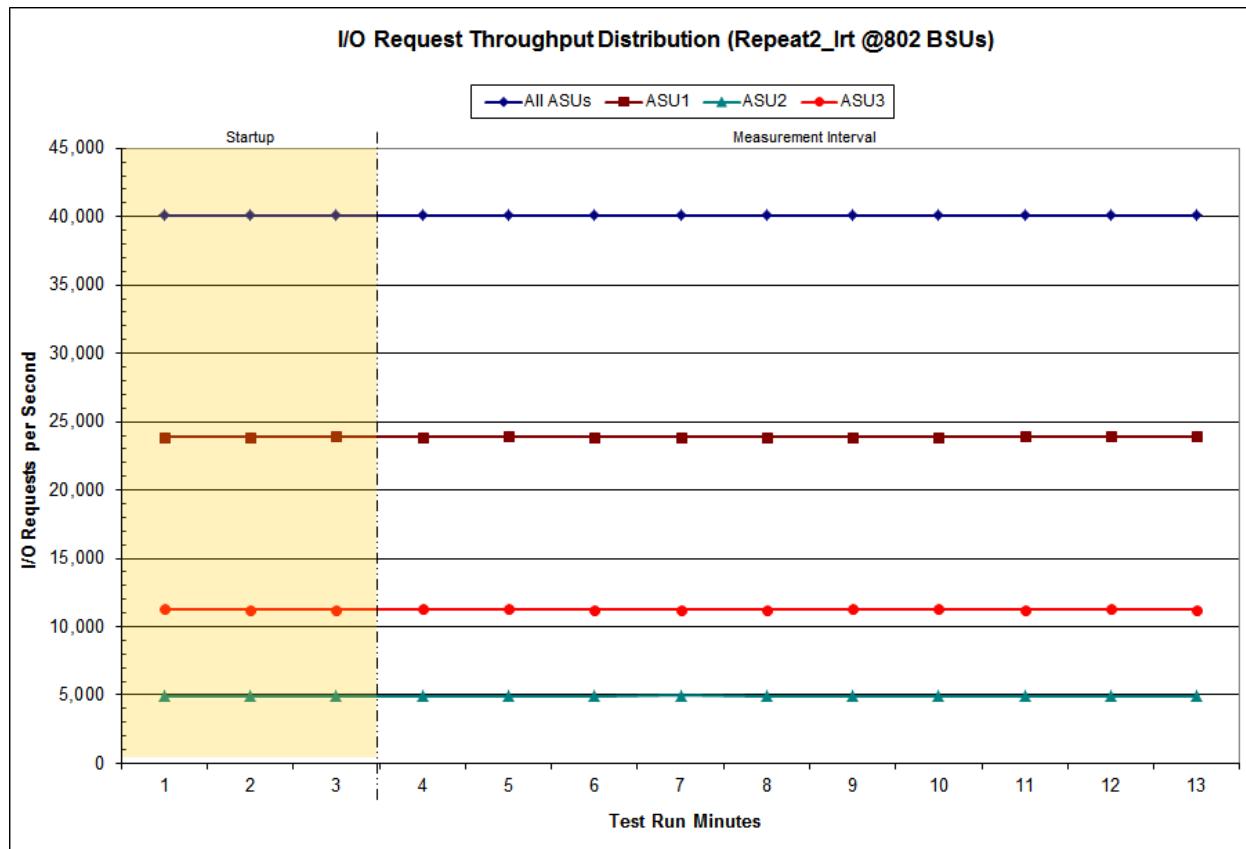

Repeatability 2 LRT –Average Response Time (ms) Distribution Data

802 BSUs	Start	Stop	Interval	Duration
<i>Start-Up/Ramp-Up</i>	14:17:54	14:20:54	0-2	0:03:00
<i>Measurement Interval</i>	14:20:54	14:30:54	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	0.37	0.36	0.38	0.38
1	0.39	0.38	0.40	0.40
2	0.38	0.37	0.40	0.38
3	0.39	0.38	0.41	0.40
4	0.38	0.38	0.40	0.39
5	0.38	0.38	0.40	0.39
6	0.39	0.38	0.41	0.40
7	0.39	0.38	0.41	0.40
8	0.38	0.38	0.40	0.38
9	0.39	0.38	0.40	0.40
10	0.38	0.38	0.40	0.39
11	0.40	0.39	0.41	0.41
12	0.39	0.38	0.41	0.40
Average	0.39	0.38	0.40	0.40


Repeatability 2 LRT –Average Response Time (ms) Distribution Graph

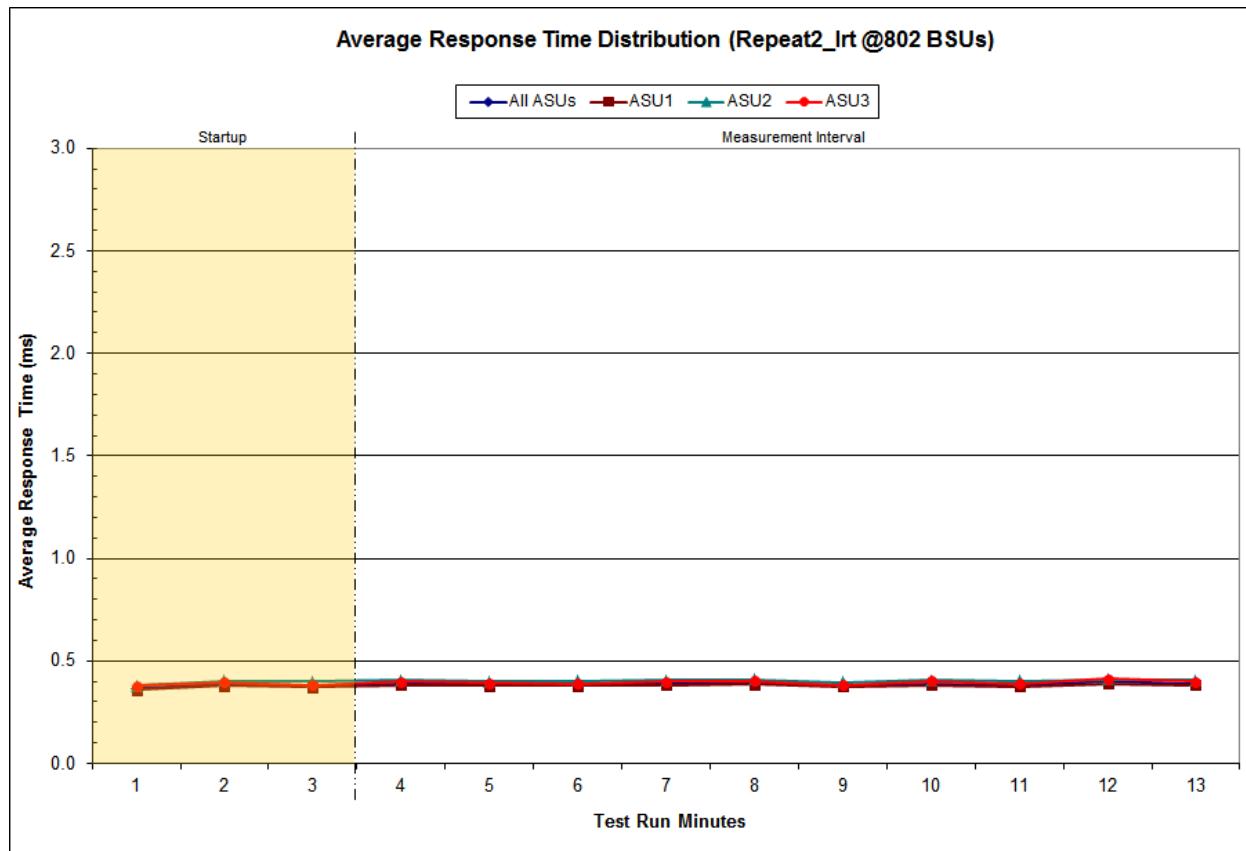

Repeatability 2 IOPS – I/O Request Throughput Distribution Data

8,020 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up	14:31:44	14:34:45	0-2	0:03:01
Measurement Interval	14:34:45	14:44:45	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	401,073.85	238,934.95	49,340.72	112,798.18
1	400,995.93	238,947.53	49,374.23	112,674.17
2	400,909.62	238,963.30	49,309.37	112,636.95
3	400,957.33	238,976.32	49,316.15	112,664.87
4	401,069.55	239,026.47	49,306.97	112,736.12
5	400,974.27	239,001.12	49,314.18	112,658.97
6	400,938.35	239,000.88	49,291.33	112,646.13
7	401,019.73	238,969.25	49,303.23	112,747.25
8	401,009.60	239,024.28	49,294.82	112,690.50
9	401,041.53	239,018.85	49,338.08	112,684.60
10	400,911.65	238,938.12	49,316.05	112,657.48
11	401,015.90	238,991.67	49,342.25	112,681.98
12	401,018.78	239,020.38	49,357.12	112,641.28
Average	400,995.67	238,996.73	49,318.02	112,680.92


Repeatability 2 IOPS – I/O Request Throughput Distribution Graph

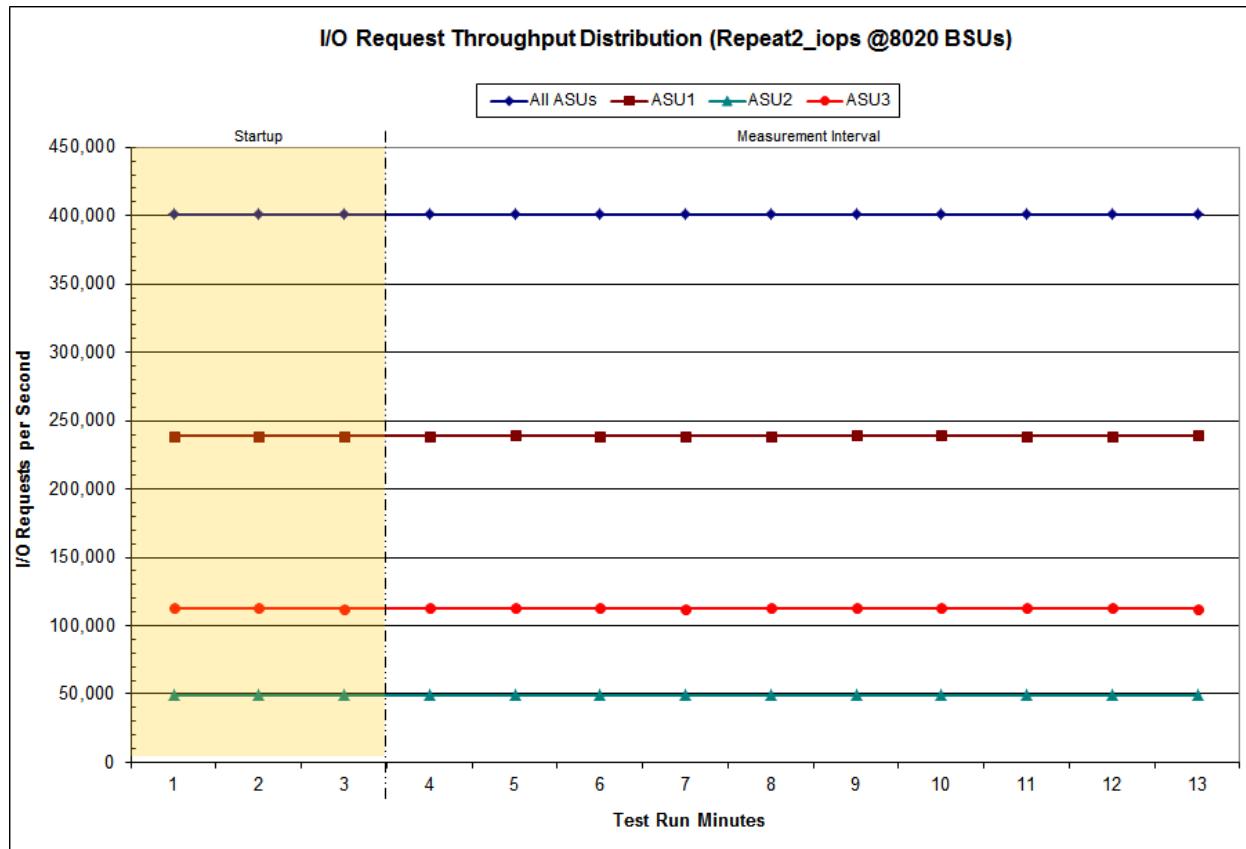

Repeatability 2 IOPS –Average Response Time (ms) Distribution Data

8,020 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up	14:31:44	14:34:45	0-2	0:03:01
Measurement Interval	14:34:45	14:44:45	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	0.82	0.88	0.92	0.65
1	0.83	0.90	0.94	0.63
2	0.82	0.90	0.93	0.62
3	0.82	0.89	0.93	0.62
4	0.84	0.91	0.94	0.64
5	0.86	0.92	0.96	0.67
6	0.82	0.90	0.93	0.61
7	0.84	0.91	0.95	0.65
8	0.84	0.91	0.94	0.64
9	0.85	0.92	0.95	0.65
10	0.88	0.95	0.98	0.70
11	0.84	0.91	0.94	0.63
12	0.83	0.91	0.94	0.63
Average	0.84	0.91	0.94	0.64

Repeatability 2 IOPS –Average Response Time (ms) Distribution Graph

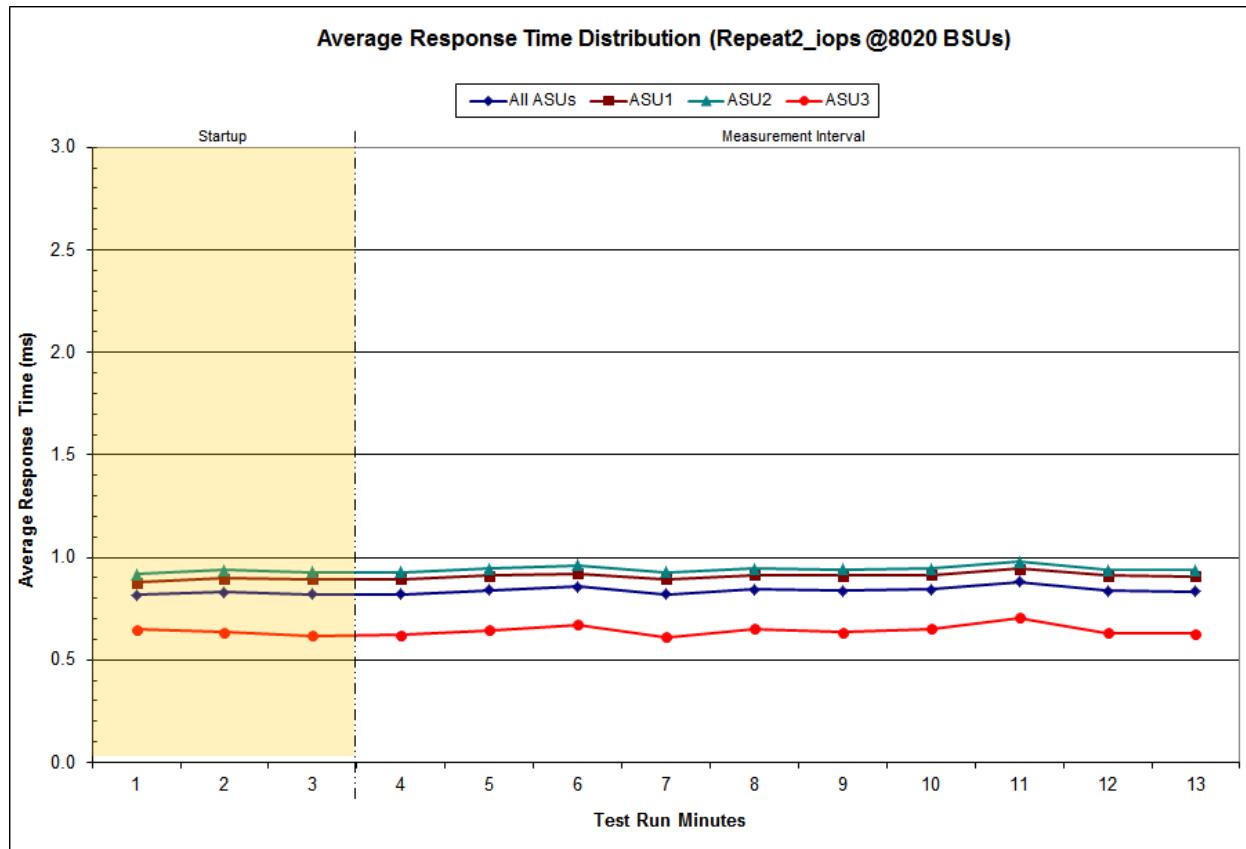

Repeatability 1 (LRT)

Measured Intensity Multiplier and Coefficient of Variation

Clause 3.4.3

IM – Intensity Multiplier: The ratio of I/Os for each I/O stream relative to the total I/Os for all I/O streams (ASU1-1 – ASU3-1) as required by the benchmark specification.

Clauses 5.1.10 and 5.3.15.2

MIM – Measured Intensity Multiplier: The Measured Intensity Multiplier represents the ratio of measured I/Os for each I/O stream relative to the total I/Os measured for all I/O streams (ASU1-1 – ASU3-1). This value may differ from the corresponding Expected Intensity Multiplier by no more than 5%.

Clause 5.3.15.3

COV – Coefficient of Variation: This measure of variation for the Measured Intensity Multiplier cannot exceed 0.2.

	ASU1-1	ASU1-2	ASU1-3	ASU1-4	ASU2-1	ASU2-2	ASU2-3	ASU3-1
IM	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
MIM	0.0350	0.2810	0.0700	0.2099	0.0180	0.0701	0.0351	0.2809
COV	0.004	0.001	0.002	0.001	0.005	0.003	0.003	0.001

Repeatability 1 (IOPS)

Measured Intensity Multiplier and Coefficient of Variation

	ASU1-1	ASU1-2	ASU1-3	ASU1-4	ASU2-1	ASU2-2	ASU2-3	ASU3-1
IM	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
MIM	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
COV	0.001	0.000	0.000	0.000	0.001	0.000	0.001	0.000

Repeatability 2 (LRT)

Measured Intensity Multiplier and Coefficient of Variation

	ASU1-1	ASU1-2	ASU1-3	ASU1-4	ASU2-1	ASU2-2	ASU2-3	ASU3-1
IM	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
MIM	0.0350	0.2809	0.0700	0.2101	0.0180	0.0701	0.0350	0.2809
COV	0.003	0.001	0.003	0.001	0.004	0.002	0.003	0.001

Repeatability 2 (IOPS)
Measured Intensity Multiplier and Coefficient of Variation

	ASU1-1	ASU1-2	ASU1-3	ASU1-4	ASU2-1	ASU2-2	ASU2-3	ASU3-1
<i>IM</i>	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
MIM	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
COV	0.001	0.000	0.000	0.000	0.001	0.001	0.001	0.000

Data Persistence Test

Clause 6

The Data Persistence Test demonstrates the Tested Storage Configuration (TSC):

- Is capable of maintaining data integrity across a power cycle.
- Ensures the transfer of data between Logical Volumes and host systems occurs without corruption or loss.

The SPC-1 Workload Generator will write 16 block I/O requests at random over the total Addressable Storage Capacity of the TSC for ten (10) minutes at a minimum of 25% of the load used to generate the SPC-1 IOPSTM primary metric. The bit pattern selected to be written to each block as well as the address of the block will be retained in a log file.

The Tested Storage Configuration (TSC) will be shutdown and restarted using a power off/power on cycle at the end of the above sequence of write operations. In addition, any caches employing battery backup must be flushed/emptied.

The SPC-1 Workload Generator will then use the above log file to verify each block written contains the correct bit pattern.

Clause 9.4.3.8

The following content shall appear in this section of the FDR:

1. A listing or screen image of all input parameters supplied to the Workload Generator.
2. For the successful Data Persistence Test Run, a table illustrating key results. The content, appearance, and format of this table are specified in Table 9-12. Information displayed in this table shall be obtained from the Test Run Results File referenced below in #3.
3. For the successful Data Persistence Test Run, the human readable Test Run Results file produced by the Workload Generator (may be contained in an appendix).

SPC-1 Workload Generator Input Parameters

The SPC-1 Workload Generator input parameters for the Sustainability, IOPS, Response Time Ramp, Repeatability, and Persistence Test Runs are documented in [Appendix E: SPC-1 Workload Generator Input Parameters](#) on Page [83](#).

Data Persistence Test Results File

A link to each test result file generated from each Data Persistence Test is listed below.

[Persistence 1 Test Results File](#)

[Persistence 2 Test Results File](#)

Data Persistence Test Results

Data Persistence Test Results	
Data Persistence Test Run Number: 1	
Total Number of Logical Blocks Written	247,287,536
Total Number of Logical Blocks Verified	160,026,432
Total Number of Logical Blocks that Failed Verification	0
Time Duration for Writing Test Logical Blocks	10 minutes
Size in bytes of each Logical Block	512
Number of Failed I/O Requests in the process of the Test	0

In some cases the same address was the target of multiple writes, which resulted in more Logical Blocks Written than Logical Blocks Verified. In the case of multiple writes to the same address, the pattern written and verified must be associated with the last write to that address.

PRICED STORAGE CONFIGURATION AVAILABILITY DATE

Clause 9.4.3.9

The committed delivery date for general availability (Availability Date) of all products that comprise the Priced Storage Configuration must be reported. When the Priced Storage Configuration includes products or components with different availability dates, the reported Availability Date for the Priced Storage Configuration must be the date at which all components are committed to be available.

The Huawei OceanStor™ 5600 V3 as documented in this Full Disclosure Report is currently available for customer purchase and shipment.

PRICING INFORMATION

Clause 9.4.3.3.6

The Executive Summary shall contain a pricing spreadsheet as documented in Clause 8.3.1.

Pricing information may be found in the Priced Storage Configuration Pricing section on page [17](#).

TESTED STORAGE CONFIGURATION (TSC) AND PRICED STORAGE CONFIGURATION DIFFERENCES

Clause 9.4.3.3.8

The Executive Summary shall contain a list of all differences between the Tested Storage Configuration (TSC) and the Priced Storage Configuration.

A list of all differences between the Tested Storage Configuration (TSC) and Priced Storage Configuration may be found in the Executive Summary portion of this document on page [17](#).

ANOMALIES OR IRREGULARITIES

Clause 9.4.3.10

The FDR shall include a clear and complete description of any anomalies or irregularities encountered in the course of executing the SPC-1 benchmark that may in any way call into question the accuracy, verifiability, or authenticity of information published in this FDR.

There were no anomalies or irregularities encountered during the SPC-1 Remote Audit of the Huawei OceanStor™ 5600 V3.

APPENDIX A: SPC-1 GLOSSARY

“Decimal” (*powers of ten*) Measurement Units

In the storage industry, the terms “kilo”, “mega”, “giga”, “tera”, “peta”, and “exa” are commonly used prefixes for computing performance and capacity. For the purposes of the SPC workload definitions, all of the following terms are defined in “powers of ten” measurement units.

A kilobyte (KB) is equal to 1,000 (10^3) bytes.

A megabyte (MB) is equal to 1,000,000 (10^6) bytes.

A gigabyte (GB) is equal to 1,000,000,000 (10^9) bytes.

A terabyte (TB) is equal to 1,000,000,000,000 (10^{12}) bytes.

A petabyte (PB) is equal to 1,000,000,000,000,000 (10^{15}) bytes

An exabyte (EB) is equal to 1,000,000,000,000,000,000 (10^{18}) bytes

“Binary” (*powers of two*) Measurement Units

The sizes reported by many operating system components use “powers of two” measurement units rather than “power of ten” units. The following standardized definitions and terms are also valid and may be used in this document.

A kibibyte (KiB) is equal to 1,024 (2^{10}) bytes.

A mebibyte (MiB) is equal to 1,048,576 (2^{20}) bytes.

A gigabyte (GiB) is equal to 1,073,741,824 (2^{30}) bytes.

A tebibyte (TiB) is equal to 1,099,511,627,776 (2^{40}) bytes.

A pebibyte (PiB) is equal to 1,125,899,906,842,624 (2^{50}) bytes.

An exbibyte (EiB) is equal to 1,152,921,504,606,846,967 (2^{60}) bytes.

SPC-1 Data Repository Definitions

Total ASU Capacity: The total storage capacity read and written in the course of executing the SPC-1 benchmark.

Application Storage Unit (ASU): The logical interface between the storage and SPC-1 Workload Generator. The three ASUs (Data, User, and Log) are typically implemented on one or more Logical Volume.

Logical Volume: The division of Addressable Storage Capacity into individually addressable logical units of storage used in the SPC-1 benchmark. Each Logical Volume is implemented as a single, contiguous address space.

Addressable Storage Capacity: The total storage (sum of Logical Volumes) that can be read and written by application programs such as the SPC-1 Workload Generator.

Configured Storage Capacity: This capacity includes the Addressable Storage Capacity and any other storage (parity disks, hot spares, etc.) necessary to implement the Addressable Storage Capacity.

Physical Storage Capacity: The formatted capacity of all storage devices physically present in the Tested Storage Configuration (TSC).

Data Protection Overhead: The storage capacity required to implement the selected level of data protection.

Required Storage: The amount of Configured Storage Capacity required to implement the Addressable Storage Configuration, excluding the storage required for the three ASUs.

Global Storage Overhead: The amount of Physical Storage Capacity that is required for storage subsystem use and unavailable for use by application programs.

Total Unused Storage: The amount of storage capacity available for use by application programs but not included in the Total ASU Capacity.

SPC-1 Data Protection Levels

Protected 1: The single point of failure of any *storage device* in the configuration will not result in permanent loss of access to or integrity of the SPC-1 Data Repository.

Protected 2: The single point of failure of any *component* in the configuration will not result in permanent loss of access to or integrity of the SPC-1 Data Repository.

SPC-1 Test Execution Definitions

Average Response Time: The sum of the Response Times for all Measured I/O Requests divided by the total number of Measured I/O Requests.

Completed I/O Request: An I/O Request with a Start Time and a Completion Time (see “I/O Completion Types” below).

Completion Time: The time recorded by the Workload Generator when an I/O Request is satisfied by the TSC as signaled by System Software.

Data Rate: The data transferred in all Measured I/O Requests in an SPC-1 Test Run divided by the length of the Test Run in seconds.

Expected I/O Count: For any given I/O Stream and Test Phase, the product of 50 times the BSU level, the duration of the Test Phase in seconds, and the Intensity Multiplier for that I/O Stream.

Failed I/O Request: Any I/O Request issued by the Workload Generator that could not be completed or was signaled as failed by System Software. A Failed I/O Request has no Completion Time (see “I/O Completion Types” below).

I/O Request Throughput: The total number of Measured I/O requests in an SPC-1 Test Run divided by the duration of the Measurement Interval in seconds.

In-Flight I/O Request: An I/O Request issued by the I/O Command Generator to the TSC that has a recorded Start Time, but does not complete within the Measurement Interval (see “I/O Completion Types” below).

Measured I/O Request: A Completed I/O Request with a Completion Time occurring within the Measurement Interval (see “I/O Completion Types” below).

Measured Intensity Multiplier: The percentage of all Measured I/O Requests that were issued by a given I/O Stream.

Measurement Interval: The finite and contiguous time period, after the TSC has reached Steady State, when data is collected by a Test Sponsor to generate an SPC-1 test result or support an SPC-1 test result.

Ramp-Up: The time required for the Benchmark Configuration (BC) to produce Steady State throughput after the Workload Generator begins submitting I/O Requests to the TSC for execution.

Ramp-Down: The time required for the BC to complete all I/O Requests issued by the Workload Generator. The Ramp-Down period begins when the Workload Generator ceases to issue new I/O Requests to the TSC.

Response Time: The Response Time of a Measured I/O Request is its Completion Time minus its Start Time.

Start Time: The time recorded by the Workload Generator when an I/O Request is submitted, by the Workload Generator, to the System Software for execution on the Tested Storage Configuration (TSC).

Start-Up: The period that begins after the Workload Generator starts to submit I/O requests to the TSC and ends at the beginning of the Measurement Interval.

Shut-Down: The period between the end of the Measurement Interval and the time when all I/O Requests issued by the Workload Generator have completed or failed.


Steady State: The consistent and sustainable throughput of the TSC. During this period the load presented to the TSC by the Workload Generator is constant.

Test: A collection of Test Phases and or Test Runs sharing a common objective.


Test Run: The execution of SPC-1 for the purpose of producing or supporting an SPC-1 test result. SPC-1 Test Runs may have a finite and measured Ramp-Up period, Start-Up period, Shut-Down period, and Ramp-Down period as illustrated in the “SPC-1 Test Run Components” below. All SPC-1 Test Runs shall have a Steady State period and a Measurement Interval.

Test Phase: A collection of one or more SPC-1 Test Runs sharing a common objective and intended to be run in a specific sequence.

I/O Completion Types

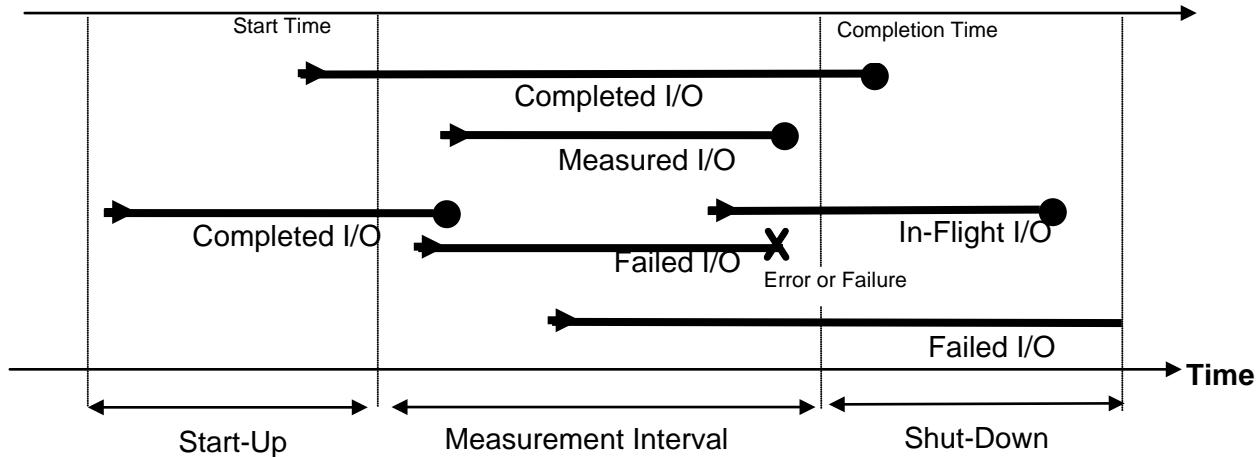

SPC-1 Test Run Components

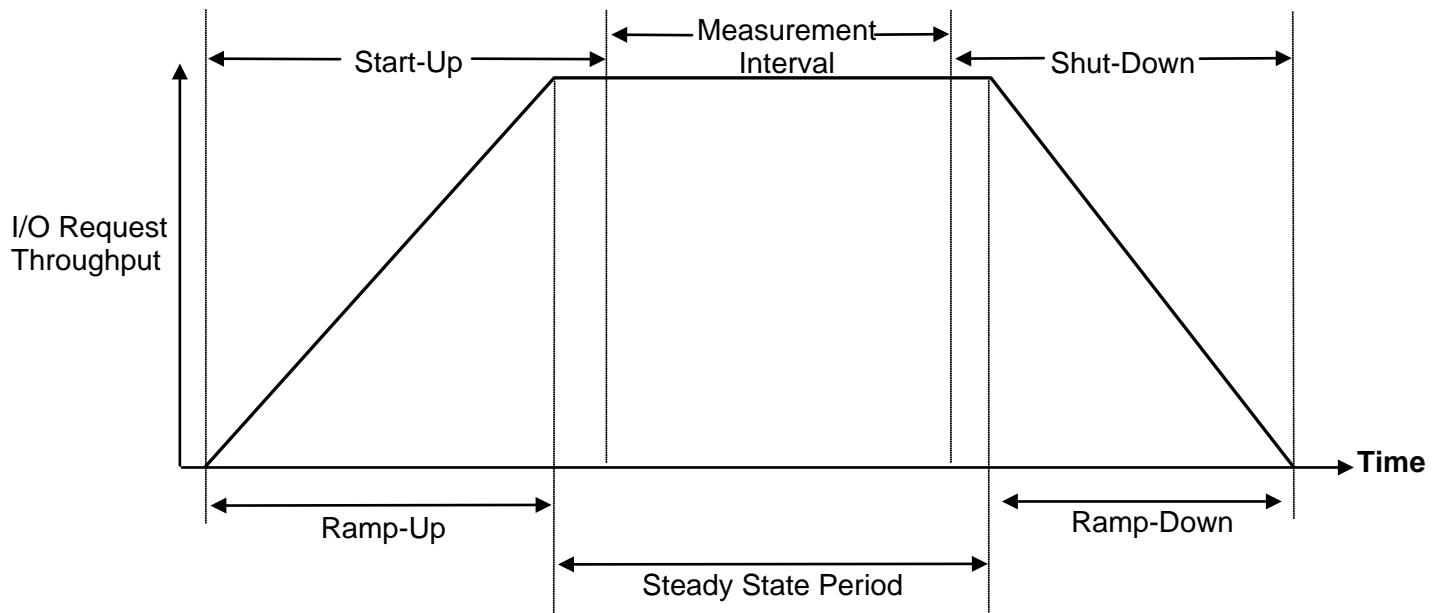

APPENDIX B: CUSTOMER TUNABLE PARAMETERS AND OPTIONS

Red Hat Enterprise Linux 7.0 (64-bit)

Change the I/O scheduler from ***cfq*** to ***noop*** on each Host System, which will result in all incoming I/O requests inserted into a simple, unordered FIFO queue. This change was done by the execution of the ***scheduler.sh*** script as documented in [*Appendix C: Tested Storage Configuration \(TSC\) Creation.*](#)

APPENDIX C: TESTED STORAGE CONFIGURATION (TSC) CREATION

The scripts referenced in Steps 2 and 3 appear in the section, [Referenced Scripts](#).

Step 1: Create Mapping View, LUN Group, Host Group and Host

Execute the following commands using the OceanStor 5600 V3 CLI from the master Host System to complete the following:

- Create one ***mapping_view (map1)***
- Create one ***lun_group (lg1)***
- Create one ***host_group (hg1)***
- Create two ***hosts (host1, host2)***
- Add ***host1*** and ***host2*** to ***hg1***
- Add ***hg1*** and ***lg1*** to ***map1***
- Add the FC ports' WWN to ***host1*** and ***host2***

```
create mapping_view name=map1 mapping_view_id=1
create lun_group name=lg1 lun_group_id=1
create host_group name=hg1 host_group_id=1
create host name=host1 operating_system=Linux host_id=1
create host name=host2 operating_system=Linux host_id=2

add host_group host host_group_id=1 host_id_list=1,2
add mapping_view host_group mapping_view_id=1 host_group_id=1
add mapping_view lun_group mapping_view_id=1 lun_group_id=1

add host initiator host_id=1 initiator_type=FC wwn=2100001b320b463e
add host initiator host_id=1 initiator_type=FC wwn=21000024ff29aff6
add host initiator host_id=1 initiator_type=FC wwn=21000024ff29aff7
add host initiator host_id=1 initiator_type=FC wwn=21000024ff2c953e
add host initiator host_id=1 initiator_type=FC wwn=21000024ff2c953f
add host initiator host_id=1 initiator_type=FC wwn=21000024ff35e744
add host initiator host_id=1 initiator_type=FC wwn=21000024ff35e745
add host initiator host_id=1 initiator_type=FC wwn=21000024ff371eec
add host initiator host_id=1 initiator_type=FC wwn=21000024ff371eed
add host initiator host_id=1 initiator_type=FC wwn=21000024ff37555c
add host initiator host_id=1 initiator_type=FC wwn=21000024ff37555d
add host initiator host_id=1 initiator_type=FC wwn=21000024ff3cb158
add host initiator host_id=1 initiator_type=FC wwn=21000024ff3cb159
add host initiator host_id=1 initiator_type=FC wwn=21000024ff3cc450
add host initiator host_id=1 initiator_type=FC wwn=21000024ff3cc451
add host initiator host_id=1 initiator_type=FC wwn=21000024ff3cc528
add host initiator host_id=2 initiator_type=FC wwn=21000024ff3cc529
add host initiator host_id=2 initiator_type=FC wwn=21000024ff455e92
add host initiator host_id=2 initiator_type=FC wwn=21000024ff455e93
```

```
add host initiator host_id=2 initiator_type=FC wwn=21000024ff49992c
add host initiator host_id=2 initiator_type=FC wwn=21000024ff49992d
add host initiator host_id=2 initiator_type=FC wwn=21000024ff4b8194
add host initiator host_id=2 initiator_type=FC wwn=21000024ff4b8195
add host initiator host_id=2 initiator_type=FC wwn=21000024ff4b829c
add host initiator host_id=2 initiator_type=FC wwn=21000024ff4b829d
add host initiator host_id=2 initiator_type=FC wwn=21000024ff4b900c
add host initiator host_id=2 initiator_type=FC wwn=21000024ff4b900d
add host initiator host_id=2 initiator_type=FC wwn=21000024ff536aea
add host initiator host_id=2 initiator_type=FC wwn=21000024ff536aeb
add host initiator host_id=2 initiator_type=FC wwn=2101001b322b463e
add host initiator host_id=2 initiator_type=FC wwn=50014380186b22fc
add host initiator host_id=2 initiator_type=FC wwn=50014380186b22fe
```

Step 2: Create Disk Domains, Storage Pools, LUNs

Execute the [**mklun.sh**](#) script on the Host System, which has **expect** installed to complete the following:

- Create 8 disk domains
- Create 8 storage pools
(*one storage pool per disk domain using all available capacity*)
- Create 16 LUNs
(*two LUNs per storage pool using all available capacity*)
- Add the 16 LUNs to **lun_group, lg1**

Note: Expect is a Unix automation and testing tool, written by Don Libes as an extension to the Tcl scripting language, for interactive applications such as telnet, ftp, passwd, fsck, rlogin, tip, ssh, and others. It uses Unix pseudo terminals to wrap up subprocesses transparently, allowing the automation of arbitrary applications that are accessed over a terminal. Expect is an open source tool can be downloaded at the following location: <http://www.nist.gov/el/msid/expect.cfm>

Step 3: Create Volumes on the Master Host System

Execute the [**mkvolume.sh**](#) script on the Master Host System to create 38 logical volumes as follows:

1. Create Physical Volume

Create 16 physical volumes using the **pvcreate** command.

2. Create Volumes Groups

Create one volume group (**vg1**) using the **vgcreate** command and the following 16 physical volumes:

/dev/sdb, /dev/sdc, /dev/sdd, /dev/sde, /dev/sdf, /dev/sdg, /dev/sdh, /dev/sdi, /dev/sdj, /dev/sdk, /dev/sdl, /dev/sdm, /dev/sdn, /dev/sdo, /dev/sdp, /dev/sdq

3. Create Logical Volumes

- Create 18 logical volumes, each with a capacity of 198 GiB, on **vg1** for ASU-1.
- Create 18 logical volumes, each with a capacity of 198 GiB, on **vg1** for ASU-2.
- Create 2 logical volumes, each with a capacity of 396 GiB, on **vg1** for ASU-3.

Step 4: Change the Scheduler on each Host System

Execute the [scheduler.sh](#) script on the Host System to change the scheduler of each block device from **cfq** to **noop**.

Referenced Scripts

mklun.sh

```
#!/bin/bash

stor=100.148.52.161
stor_user=admin
stor_pswd=Admin@storage1

export LANG=C

echo "creating LUN ..."

expect <<__END_CREATE_LUN
spawn ssh $stor_user@$stor
set timeout 60
expect {
    -re "assword" { send "$stor_pswd\r" }
    -re "yes/no" { send "yes\r"; exp_continue }
}
expect ">

# -----create disk_domain-----
send "create disk_domain name=ASU000 disk_list=DAE000.0-7 disk_domain_id=0\r"
expect ">"
send "create disk_domain name=ASU001 disk_list=DAE000.8-15 disk_domain_id=1\r"
expect ">"
send "create disk_domain name=ASU002 disk_list=DAE040.0-7 disk_domain_id=2\r"
expect ">"
send "create disk_domain name=ASU003 disk_list=DAE040.8-15 disk_domain_id=3\r"
expect ">"
send "create disk_domain name=ASU100 disk_list=DAE100.0-7 disk_domain_id=4\r"
expect ">"
send "create disk_domain name=ASU101 disk_list=DAE100.8-15 disk_domain_id=5\r"
expect ">"
send "create disk_domain name=ASU102 disk_list=DAE140.0-7 disk_domain_id=6\r"
expect ">"
send "create disk_domain name=ASU103 disk_list=DAE140.8-15 disk_domain_id=7\r"
expect ">

# -----create storage_pool -----
send "create storage_pool name=ASU000 disk_type=SSD capacity=1236GB pool_id=0
disk_domain_id=0 raid_level=RAID10 stripe_depth=32KB\r"
expect ">"
```

```
send "create storage_pool name=ASU001 disk_type=SSD capacity=1253GB pool_id=1
disk_domain_id=1 raid_level=RAID10 stripe_depth=32KB\r"
expect ">"
send "create storage_pool name=ASU002 disk_type=SSD capacity=1253GB pool_id=2
disk_domain_id=2 raid_level=RAID10 stripe_depth=32KB\r"
expect ">"
send "create storage_pool name=ASU003 disk_type=SSD capacity=1253GB pool_id=3
disk_domain_id=3 raid_level=RAID10 stripe_depth=32KB\r"
expect ">"
send "create storage_pool name=ASU100 disk_type=SSD capacity=1236GB pool_id=4
disk_domain_id=4 raid_level=RAID10 stripe_depth=32KB\r"
expect ">"
send "create storage_pool name=ASU101 disk_type=SSD capacity=1253GB pool_id=5
disk_domain_id=5 raid_level=RAID10 stripe_depth=32KB\r"
expect ">"
send "create storage_pool name=ASU102 disk_type=SSD capacity=1253GB pool_id=6
disk_domain_id=6 raid_level=RAID10 stripe_depth=32KB\r"
expect ">"
send "create storage_pool name=ASU103 disk_type=SSD capacity=1253GB pool_id=7
disk_domain_id=7 raid_level=RAID10 stripe_depth=32KB\r"
expect ">"

# -----create lun -----
send "create lun name=ASU000 pool_id=0 capacity=617GB owner_controller=0A
lun_id=0\r"
expect ">"
send "create lun name=ASU001 pool_id=0 capacity=617GB owner_controller=0B
lun_id=1\r"
expect ">"
send "create lun name=ASU002 pool_id=1 capacity=626GB owner_controller=0A
lun_id=2\r"
expect ">"
send "create lun name=ASU003 pool_id=1 capacity=626GB owner_controller=0B
lun_id=3\r"
expect ">"
send "create lun name=ASU004 pool_id=2 capacity=626GB owner_controller=0A
lun_id=4\r"
expect ">"
send "create lun name=ASU005 pool_id=2 capacity=626GB owner_controller=0B
lun_id=5\r"
expect ">"
send "create lun name=ASU006 pool_id=3 capacity=626GB owner_controller=0A
lun_id=6\r"
expect ">"
send "create lun name=ASU007 pool_id=3 capacity=626GB owner_controller=0B
lun_id=7\r"
expect ">"
send "create lun name=ASU100 pool_id=4 capacity=617GB owner_controller=1A
lun_id=8\r"
expect ">"
send "create lun name=ASU101 pool_id=4 capacity=617GB owner_controller=1B
lun_id=9\r"
expect ">"
send "create lun name=ASU102 pool_id=5 capacity=626GB owner_controller=1A
lun_id=10\r"
expect ">"
send "create lun name=ASU103 pool_id=5 capacity=626GB owner_controller=1B
lun_id=11\r"
expect ">"
send "create lun name=ASU104 pool_id=6 capacity=626GB owner_controller=1A
lun_id=12\r"
expect ">"
```

```
send "create lun name=ASU105 pool_id=6 capacity=626GB owner_controller=1B
lun_id=13\r"
expect ">"
send "create lun name=ASU106 pool_id=7 capacity=626GB owner_controller=1A
lun_id=14\r"
expect ">"
send "create lun name=ASU107 pool_id=7 capacity=626GB owner_controller=1B
lun_id=15\r"
expect ">"

# ----- add all luns to lun_group-----
send "add lun_group lun lun_group_id=1
lun_id_list=0,1,8,9,2,3,10,11,4,5,12,13,6,7,14,15"
expect ">

send "exit\r"
expect "(y/n):"
send "y\r"
expect EOF
__END_CREATE_LUN
```

mkvolume.sh

```
pvcreate /dev/sdb
pvcreate /dev/sdc
pvcreate /dev/sdd
pvcreate /dev/sde
pvcreate /dev/sdf
pvcreate /dev/sdg
pvcreate /dev/sdh
pvcreate /dev/sdi
pvcreate /dev/sdj
pvcreate /dev/sdk
pvcreate /dev/sdl
pvcreate /dev/sdm
pvcreate /dev/sdn
pvcreate /dev/sdo
pvcreate /dev/sdp
pvcreate /dev/sdq

vgcreate vg1 /dev/sdb /dev/sdc /dev/sdd /dev/sde /dev/sdf /dev/sdg /dev/sdh /dev/sdi
/dev/sdj /dev/sdk /dev/sdl /dev/sdm /dev/sdn /dev/sdo /dev/sdp /dev/sdq

lvcreate -n asul01 -i 16 -I 512 -C y -L 198g vg1
lvcreate -n asul02 -i 16 -I 512 -C y -L 198g vg1
lvcreate -n asul03 -i 16 -I 512 -C y -L 198g vg1
lvcreate -n asul04 -i 16 -I 512 -C y -L 198g vg1
lvcreate -n asul05 -i 16 -I 512 -C y -L 198g vg1
lvcreate -n asul06 -i 16 -I 512 -C y -L 198g vg1
lvcreate -n asul07 -i 16 -I 512 -C y -L 198g vg1
lvcreate -n asul08 -i 16 -I 512 -C y -L 198g vg1
lvcreate -n asul09 -i 16 -I 512 -C y -L 198g vg1
lvcreate -n asul10 -i 16 -I 512 -C y -L 198g vg1
lvcreate -n asul11 -i 16 -I 512 -C y -L 198g vg1
lvcreate -n asul12 -i 16 -I 512 -C y -L 198g vg1
lvcreate -n asul13 -i 16 -I 512 -C y -L 198g vg1
lvcreate -n asul14 -i 16 -I 512 -C y -L 198g vg1
lvcreate -n asul15 -i 16 -I 512 -C y -L 198g vg1
lvcreate -n asul16 -i 16 -I 512 -C y -L 198g vg1
```

```
lvcreate -n asu117 -i 16 -I 512 -C y -L 198g vgl  
lvcreate -n asu118 -i 16 -I 512 -C y -L 198g vgl  
  
lvcreate -n asu201 -i 16 -I 512 -C y -L 198g vgl  
lvcreate -n asu202 -i 16 -I 512 -C y -L 198g vgl  
lvcreate -n asu203 -i 16 -I 512 -C y -L 198g vgl  
lvcreate -n asu204 -i 16 -I 512 -C y -L 198g vgl  
lvcreate -n asu205 -i 16 -I 512 -C y -L 198g vgl  
lvcreate -n asu206 -i 16 -I 512 -C y -L 198g vgl  
lvcreate -n asu207 -i 16 -I 512 -C y -L 198g vgl  
lvcreate -n asu208 -i 16 -I 512 -C y -L 198g vgl  
lvcreate -n asu209 -i 16 -I 512 -C y -L 198g vgl  
lvcreate -n asu210 -i 16 -I 512 -C y -L 198g vgl  
lvcreate -n asu211 -i 16 -I 512 -C y -L 198g vgl  
lvcreate -n asu212 -i 16 -I 512 -C y -L 198g vgl  
lvcreate -n asu213 -i 16 -I 512 -C y -L 198g vgl  
lvcreate -n asu214 -i 16 -I 512 -C y -L 198g vgl  
lvcreate -n asu215 -i 16 -I 512 -C y -L 198g vgl  
lvcreate -n asu216 -i 16 -I 512 -C y -L 198g vgl  
lvcreate -n asu217 -i 16 -I 512 -C y -L 198g vgl  
lvcreate -n asu218 -i 16 -I 512 -C y -L 198g vgl  
  
lvcreate -n asu301 -i 16 -I 512 -C y -L 396g vgl  
lvcreate -n asu302 -i 16 -I 512 -C y -L 396g vgl
```

scheduler.sh

```
echo noop > /sys/block/sdb/queue/scheduler  
echo noop > /sys/block/sdc/queue/scheduler  
echo noop > /sys/block/sdd/queue/scheduler  
echo noop > /sys/block/sde/queue/scheduler  
echo noop > /sys/block/sdf/queue/scheduler  
echo noop > /sys/block/sdg/queue/scheduler  
echo noop > /sys/block/sdh/queue/scheduler  
echo noop > /sys/block/sdi/queue/scheduler  
echo noop > /sys/block/sdj/queue/scheduler  
echo noop > /sys/block/sdk/queue/scheduler  
echo noop > /sys/block/sdl/queue/scheduler  
echo noop > /sys/block/sdm/queue/scheduler  
echo noop > /sys/block/sdo/queue/scheduler  
echo noop > /sys/block/sdp/queue/scheduler  
echo noop > /sys/block/sdq/queue/scheduler
```

APPENDIX D: SPC-1 WORKLOAD GENERATOR STORAGE COMMANDS AND PARAMETERS

ASU Pre-Fill

```
compratio=1
hd=default,vdbench=/root/vdbench,user=root,shell=ssh

hd=hd1,system=host1
hd=hd2,system=host2

sd=default,openflags=o_direct,threads=8

sd=sd1,host=hd1,lun=/dev/vg1/asu101,size=212600881152
sd=sd2,host=hd1,lun=/dev/vg1/asu102,size=212600881152
sd=sd3,host=hd1,lun=/dev/vg1/asu103,size=212600881152
sd=sd4,host=hd1,lun=/dev/vg1/asu104,size=212600881152
sd=sd5,host=hd2,lun=/dev/vg1/asu105,size=212600881152
sd=sd6,host=hd2,lun=/dev/vg1/asu106,size=212600881152
sd=sd7,host=hd2,lun=/dev/vg1/asu107,size=212600881152
sd=sd8,host=hd2,lun=/dev/vg1/asu108,size=212600881152
sd=sd9,host=hd1,lun=/dev/vg1/asu109,size=212600881152
sd=sd10,host=hd1,lun=/dev/vg1/asu110,size=212600881152
sd=sd11,host=hd1,lun=/dev/vg1/asu111,size=212600881152
sd=sd12,host=hd1,lun=/dev/vg1/asu112,size=212600881152
sd=sd13,host=hd2,lun=/dev/vg1/asu113,size=212600881152
sd=sd14,host=hd2,lun=/dev/vg1/asu114,size=212600881152
sd=sd15,host=hd2,lun=/dev/vg1/asu115,size=212600881152
sd=sd16,host=hd2,lun=/dev/vg1/asu116,size=212600881152
sd=sd17,host=hd1,lun=/dev/vg1/asu117,size=212600881152
sd=sd18,host=hd1,lun=/dev/vg1/asu118,size=212600881152

sd=sd19,host=hd1,lun=/dev/vg1/asu201,size=212600881152
sd=sd20,host=hd1,lun=/dev/vg1/asu202,size=212600881152
sd=sd21,host=hd2,lun=/dev/vg1/asu203,size=212600881152
sd=sd22,host=hd2,lun=/dev/vg1/asu204,size=212600881152
sd=sd23,host=hd2,lun=/dev/vg1/asu205,size=212600881152
sd=sd24,host=hd2,lun=/dev/vg1/asu206,size=212600881152
sd=sd25,host=hd1,lun=/dev/vg1/asu207,size=212600881152
sd=sd26,host=hd1,lun=/dev/vg1/asu208,size=212600881152
sd=sd27,host=hd1,lun=/dev/vg1/asu209,size=212600881152
sd=sd28,host=hd1,lun=/dev/vg1/asu210,size=212600881152
sd=sd29,host=hd2,lun=/dev/vg1/asu211,size=212600881152
sd=sd30,host=hd2,lun=/dev/vg1/asu212,size=212600881152
sd=sd31,host=hd2,lun=/dev/vg1/asu213,size=212600881152
sd=sd32,host=hd2,lun=/dev/vg1/asu214,size=212600881152
sd=sd33,host=hd1,lun=/dev/vg1/asu215,size=212600881152
sd=sd34,host=hd1,lun=/dev/vg1/asu216,size=212600881152
sd=sd35,host=hd1,lun=/dev/vg1/asu217,size=212600881152
sd=sd36,host=hd1,lun=/dev/vg1/asu218,size=212600881152

sd=sd37,host=hd2,lun=/dev/vg1/asu301,size=425201762304
sd=sd38,host=hd2,lun=/dev/vg1/asu302,size=425201762304

wd=wd1,sd=sd*,rdpct=0,seekpct=-1,xfersize=1024K
rd=PREPASU1,wd=wd1,iorate=max,elapsed=3600000,interval=10
```

Primary Metrics and Repeatability Tests

The content of SPC-1 Workload Generator command and parameter file used in this benchmark to execute the Primary Metrics (*Sustainability Test Phase, IOPS Test Phase, and Response Time Ramp Test Phase*) and Repeatability (*Repeatability Test Phase 1 and Repeatability Test Phase 2*) Tests is listed below.

```
host=master
slaves=(slave1,slave2,slave3,slave4,slave5,slave6,slave7,slave8,slave9,slave10,slave
11,slave12,slave13,slave14,slave15,slave16,slave17,slave18,slave19,slave20,slave21,s
lave22,slave23,slave24,slave25,slave26,slave27,slave28,slave29,slave30,slave31,slave
32,slave33,slave34,slave35,slave36,slave37,slave38,slave39,slave40,slave41,slave42,s
lave43,slave44,slave45,slave46,slave47,slave48,slave49,slave50,slave51,slave52,slave
53,slave54,slave55,slave56,slave57,slave58,slave59,slave60,slave61,slave62,slave63,s
lave64,slave65,slave66,slave67,slave68,slave69,slave70,slave71,slave72,slave73,slave
74,slave75,slave76,slave77,slave78,slave79,slave80,slave81,slave82)

sd=asu1_1,lun=/dev/vg1/asu101,size=212600881152
sd=asu1_2,lun=/dev/vg1/asu102,size=212600881152
sd=asu1_3,lun=/dev/vg1/asu103,size=212600881152
sd=asu1_4,lun=/dev/vg1/asu104,size=212600881152
sd=asu1_5,lun=/dev/vg1/asu105,size=212600881152
sd=asu1_6,lun=/dev/vg1/asu106,size=212600881152
sd=asu1_7,lun=/dev/vg1/asu107,size=212600881152
sd=asu1_8,lun=/dev/vg1/asu108,size=212600881152
sd=asu1_9,lun=/dev/vg1/asu109,size=212600881152
sd=asu1_10,lun=/dev/vg1/asu110,size=212600881152
sd=asu1_11,lun=/dev/vg1/asu111,size=212600881152
sd=asu1_12,lun=/dev/vg1/asu112,size=212600881152
sd=asu1_13,lun=/dev/vg1/asu113,size=212600881152
sd=asu1_14,lun=/dev/vg1/asu114,size=212600881152
sd=asu1_15,lun=/dev/vg1/asu115,size=212600881152
sd=asu1_16,lun=/dev/vg1/asu116,size=212600881152
sd=asu1_17,lun=/dev/vg1/asu117,size=212600881152
sd=asu1_18,lun=/dev/vg1/asu118,size=212600881152

sd=asu2_1,lun=/dev/vg1/asu201,size=212600881152
sd=asu2_2,lun=/dev/vg1/asu202,size=212600881152
sd=asu2_3,lun=/dev/vg1/asu203,size=212600881152
sd=asu2_4,lun=/dev/vg1/asu204,size=212600881152
sd=asu2_5,lun=/dev/vg1/asu205,size=212600881152
sd=asu2_6,lun=/dev/vg1/asu206,size=212600881152
sd=asu2_7,lun=/dev/vg1/asu207,size=212600881152
sd=asu2_8,lun=/dev/vg1/asu208,size=212600881152
sd=asu2_9,lun=/dev/vg1/asu209,size=212600881152
sd=asu2_10,lun=/dev/vg1/asu210,size=212600881152
sd=asu2_11,lun=/dev/vg1/asu211,size=212600881152
sd=asu2_12,lun=/dev/vg1/asu212,size=212600881152
sd=asu2_13,lun=/dev/vg1/asu213,size=212600881152
sd=asu2_14,lun=/dev/vg1/asu214,size=212600881152
sd=asu2_15,lun=/dev/vg1/asu215,size=212600881152
sd=asu2_16,lun=/dev/vg1/asu216,size=212600881152
sd=asu2_17,lun=/dev/vg1/asu217,size=212600881152
sd=asu2_18,lun=/dev/vg1/asu218,size=212600881152

sd=asu3_1,lun=/dev/vg1/asu301,size=425201762304
sd=asu3_2,lun=/dev/vg1/asu302,size=425201762304
```

SPC-1 Persistence

The content of SPC-1 Workload Generator command and parameter file, used in this benchmark to execute the SPC-1 Persistence Test, is listed below.

```
sd=asu1_1,lun=/dev/vg1/asu101,size=212600881152
sd=asu1_2,lun=/dev/vg1/asu102,size=212600881152
sd=asu1_3,lun=/dev/vg1/asu103,size=212600881152
sd=asu1_4,lun=/dev/vg1/asu104,size=212600881152
sd=asu1_5,lun=/dev/vg1/asu105,size=212600881152
sd=asu1_6,lun=/dev/vg1/asu106,size=212600881152
sd=asu1_7,lun=/dev/vg1/asu107,size=212600881152
sd=asu1_8,lun=/dev/vg1/asu108,size=212600881152
sd=asu1_9,lun=/dev/vg1/asu109,size=212600881152
sd=asu1_10,lun=/dev/vg1/asu110,size=212600881152
sd=asu1_11,lun=/dev/vg1/asu111,size=212600881152
sd=asu1_12,lun=/dev/vg1/asu112,size=212600881152
sd=asu1_13,lun=/dev/vg1/asu113,size=212600881152
sd=asu1_14,lun=/dev/vg1/asu114,size=212600881152
sd=asu1_15,lun=/dev/vg1/asu115,size=212600881152
sd=asu1_16,lun=/dev/vg1/asu116,size=212600881152
sd=asu1_17,lun=/dev/vg1/asu117,size=212600881152
sd=asu1_18,lun=/dev/vg1/asu118,size=212600881152

sd=asu2_1,lun=/dev/vg1/asu201,size=212600881152
sd=asu2_2,lun=/dev/vg1/asu202,size=212600881152
sd=asu2_3,lun=/dev/vg1/asu203,size=212600881152
sd=asu2_4,lun=/dev/vg1/asu204,size=212600881152
sd=asu2_5,lun=/dev/vg1/asu205,size=212600881152
sd=asu2_6,lun=/dev/vg1/asu206,size=212600881152
sd=asu2_7,lun=/dev/vg1/asu207,size=212600881152
sd=asu2_8,lun=/dev/vg1/asu208,size=212600881152
sd=asu2_9,lun=/dev/vg1/asu209,size=212600881152
sd=asu2_10,lun=/dev/vg1/asu210,size=212600881152
sd=asu2_11,lun=/dev/vg1/asu211,size=212600881152
sd=asu2_12,lun=/dev/vg1/asu212,size=212600881152
sd=asu2_13,lun=/dev/vg1/asu213,size=212600881152
sd=asu2_14,lun=/dev/vg1/asu214,size=212600881152
sd=asu2_15,lun=/dev/vg1/asu215,size=212600881152
sd=asu2_16,lun=/dev/vg1/asu216,size=212600881152
sd=asu2_17,lun=/dev/vg1/asu217,size=212600881152
sd=asu2_18,lun=/dev/vg1/asu218,size=212600881152

sd=asu3_1,lun=/dev/vg1/asu301,size=425201762304
sd=asu3_2,lun=/dev/vg1/asu302,size=425201762304
```

APPENDIX E: SPC-1 WORKLOAD GENERATOR INPUT PARAMETERS

The following script, **run.sh**, was invoked to execute the following in an uninterrupted execution sequence:

- Generate the first set of detailed storage configuration information required for a remote audit.
- The required ASU pre-fill.
- Start the Slave JVMs on the two Host Systems
- The commands to execute the Primary Metrics Test (*Sustainability Test Phase, IOPS Test Phase, and Response Time Ramp Test Phase*), Repeatability Test (*Repeatability Test Phase 1 and Repeatability Test Phase 2*), and SPC-1 Persistence Test Run 1 (*write phase*).

After the above test sequence completed, the script paused until the required TSC power off/power on cycle completed then executed the following:

- Generate the second set of detailed storage configuration information required for a remote audit.
- The command to execute the SPC-2 Persistence Test Run 2 (*read phase*).

run.sh

```
#!/bin/sh

#JAVA="/usr/java/jre1.6.0_45/bin/java -d64 -Xms7168m -Xmx7168m -Xmn1792m -Xss192k -Xincgc"
JAVA="/usr/java/jre1.6.0_45/bin/java -Xmx7168m -Xincgc"
EXEDIR=/root/5600

expect shstorage.tcl > profile1_storage.log
date > profile1_volume.log
lvdisplay >> profile1_volume.log
date >> profile1_volume.log

echo "ASU prefill started....."
../vdbench/vdbench -f /root/5600/prefilling.cfg -o /root/5600/PreFill
echo "ASU prefill complete....."

N=1
for host in host1 host2
do
    ssh $host rm -rf $EXEDIR/output
    ssh $host rm -rf $EXEDIR/config
    ssh $host mkdir $EXEDIR/output
    ssh $host mkdir $EXEDIR/config
    for((i=1;i<=41;i++))
    do
        echo "start slave$N on $host"
        echo "master=host1" > $EXEDIR/config/slave$N.cfg
        echo "host=slave$N" >> $EXEDIR/config/slave$N.cfg

        echo "sd=asul_1,lun=/dev/vg1/asu101,size=212600881152" >> $EXEDIR/config/slave$N.cfg
        echo "sd=asul_2,lun=/dev/vg1/asu102,size=212600881152" >> $EXEDIR/config/slave$N.cfg
        echo "sd=asul_3,lun=/dev/vg1/asu103,size=212600881152" >> $EXEDIR/config/slave$N.cfg
        echo "sd=asul_4,lun=/dev/vg1/asu104,size=212600881152" >> $EXEDIR/config/slave$N.cfg
```

```

echo "sd=asu1_5,lun=/dev/vg1/asu105,size=212600881152" >> $EXEDIR/config/slave$N.cfg
echo "sd=asu1_6,lun=/dev/vg1/asu106,size=212600881152" >> $EXEDIR/config/slave$N.cfg
echo "sd=asu1_7,lun=/dev/vg1/asu107,size=212600881152" >> $EXEDIR/config/slave$N.cfg
echo "sd=asu1_8,lun=/dev/vg1/asu108,size=212600881152" >> $EXEDIR/config/slave$N.cfg
echo "sd=asu1_9,lun=/dev/vg1/asu109,size=212600881152" >> $EXEDIR/config/slave$N.cfg
echo "sd=asu1_10,lun=/dev/vg1/asu110,size=212600881152" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu1_11,lun=/dev/vg1/asu111,size=212600881152" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu1_12,lun=/dev/vg1/asu112,size=212600881152" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu1_13,lun=/dev/vg1/asu113,size=212600881152" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu1_14,lun=/dev/vg1/asu114,size=212600881152" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu1_15,lun=/dev/vg1/asu115,size=212600881152" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu1_16,lun=/dev/vg1/asu116,size=212600881152" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu1_17,lun=/dev/vg1/asu117,size=212600881152" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu1_18,lun=/dev/vg1/asu118,size=212600881152" >>
$EXEDIR/config/slave$N.cfg

echo "sd=asu2_1,lun=/dev/vg1/asu201,size=212600881152" >> $EXEDIR/config/slave$N.cfg
echo "sd=asu2_2,lun=/dev/vg1/asu202,size=212600881152" >> $EXEDIR/config/slave$N.cfg
echo "sd=asu2_3,lun=/dev/vg1/asu203,size=212600881152" >> $EXEDIR/config/slave$N.cfg
echo "sd=asu2_4,lun=/dev/vg1/asu204,size=212600881152" >> $EXEDIR/config/slave$N.cfg
echo "sd=asu2_5,lun=/dev/vg1/asu205,size=212600881152" >> $EXEDIR/config/slave$N.cfg
echo "sd=asu2_6,lun=/dev/vg1/asu206,size=212600881152" >> $EXEDIR/config/slave$N.cfg
echo "sd=asu2_7,lun=/dev/vg1/asu207,size=212600881152" >> $EXEDIR/config/slave$N.cfg
echo "sd=asu2_8,lun=/dev/vg1/asu208,size=212600881152" >> $EXEDIR/config/slave$N.cfg
echo "sd=asu2_9,lun=/dev/vg1/asu209,size=212600881152" >> $EXEDIR/config/slave$N.cfg
echo "sd=asu2_10,lun=/dev/vg1/asu210,size=212600881152" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_11,lun=/dev/vg1/asu211,size=212600881152" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_12,lun=/dev/vg1/asu212,size=212600881152" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_13,lun=/dev/vg1/asu213,size=212600881152" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_14,lun=/dev/vg1/asu214,size=212600881152" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_15,lun=/dev/vg1/asu215,size=212600881152" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_16,lun=/dev/vg1/asu216,size=212600881152" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_17,lun=/dev/vg1/asu217,size=212600881152" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_18,lun=/dev/vg1/asu218,size=212600881152" >>
$EXEDIR/config/slave$N.cfg

echo "sd=asu3_1,lun=/dev/vg1/asu301,size=425201762304" >> $EXEDIR/config/slave$N.cfg
echo "sd=asu3_2,lun=/dev/vg1/asu302,size=425201762304" >> $EXEDIR/config/slave$N.cfg

scp $EXEDIR/config/slave$N.cfg $host:$EXEDIR/config/slave$N.cfg
ssh $host "$JAVA -cp $EXEDIR/../spcl spcl -f $EXEDIR/config/slave$N.cfg -o
$EXEDIR/output/slave$N" > /dev/null &
N=${[N+1]}
done
done

rm -rf spcl.cfg

```

```
cp metrics.cfg spc1.cfg

$JAVA -cp ../spc1 metrics -b 8020 -t 28800
$JAVA -cp ../spc1 repeat1 -b 8020
$JAVA -cp ../spc1 repeat2 -b 8020

for host in host2 host1
do
    ssh $host pkill -9 java
done

rm -rf spc1.cfg
cp persist.cfg spc1.cfg

$JAVA -cp ../spc1 persist1 -b 8020

echo "Power cycle TSC, then Enter to continue"
read

expect shstorage.tcl > profile2_storage.log
date > profile2_volume.log
lvdisplay >> profile2_volume.log
date >> profile2_volume.log

$JAVA -cp ../spc1 persist2
```

APPENDIX F: THIRD-PARTY QUOTATION

Priced Storage Configuration



Netfast Technology Solutions, Inc.

989, Avenues of America, Fl 12

New York, NY 10018, USA

Voice: (212) 792-5200 , Fax: (212) 213-1152

03/26/2016, Quote Valid:90 Days

No.	Model	Description	Qty.	Unit Price (USD)	Total Price (USD)
1	Phase				
1	Location				
1.1	OceanStor 5600 V3 Storage System				
1.1.1	Engine				
	5600V3-128G-AC	5600 V3(3U,Dual Ctrl,AC,128GB,SPE62C0300)	2	16,804.32	33,608.64
1.1.2	Expand Interface Module				
	SMARTIO8FC	4 port SmartIO I/O module(SFP+,8Gb FC)	8	665.04	5,320.32
	SMARTIO10ETH	4 port SmartIO I/O module(SFP+,10Gb Eth/FCoE(VN2VF)/Scale-out)	4	1,310.16	5,240.64
	LPU4S12V3	4 port 4*12Gb SAS I/O module(MiniSAS HD)	8	992.64	7,941.12
1.1.3	Disk Components				
	SSDM-400G2S-A1	SSD Midrange 400GB 2.5" SAS 6G Disk Unit	64	710.40	45,465.60
1.1.4	Disk Enclosure				
	DAE22525U2-1-AC	Disk Enclosure(2U,AC,2.5",Expanding Module,25 Disk Slots,without Disk Unit, DAE22525U2)	4	2,116.80	8,467.20
1.1.5	Installation Material				
	SN2F01FCPC	Patch Cord,DLC/PC,DLC/PC,Multi-mode,3m,A1a.2,2mm,OM3 bending insensitive	40	11.00	440.00
1.1.6	HBA				
	N8GHBA000	QLOGIC QLE2562 HBA Card,PCIE,8Gbps DualPort ,Fiber Channel Multimode LC Optic Interface,English Manual, No Drive CD	16	1,000.00	16,000.00
1.1.7	Storage Software				
	LIC-5600V3-BS	Basic Software License for Block(Include Device Management,SmartThin,SmartMulti-tenant,SmartMigration,SmartErase,SmartMotion,Cloud Service)	1	1,970.16	1,970.16
	LIC-5500V3-PATH	OceanStor HW UltraPath Software License	1	945.60	945.60
Total of Product					125,399.28

Priced Storage Configuration (*continued*)



Netfast Technology Solutions, Inc.

989, Avenues of America, Fl 12

New York, NY 10018, USA

Voice: (212) 792-5200 , Fax: (212) 213-1152

03/26/2016, Quote Valid:90 Days

No.	Model	Description	Qty.	Unit Price (USD)	Total Price (USD)
1.1.8					
1.1.8	Maintenance Support Service				
	02359805-88134ULJ-3	5600 V3(3U,Dual Ctrl,AC,128GB,SPE62C0300)-Warranty Upgrade To Hi-Care Onsite Premier 24x7x4H Engineer Onsite Service-3Year(s)	2	3,790.01	7,580.02
	02359806-88134ULJ-3	Disk Enclosure(2U,AC,2.5",Expanding Module,25 Disk Slots,without Disk Unit,DAE22525U2)-Warranty Upgrade To Hi-Care Onsite Premier 24x7x4H Engineer Onsite Service-3Year(s)	3	2,440.01	7,320.03
	88032QRN-88134UHK-3	OceanStor HW UltraPath Software License-Hi-Care Application Software Upgrade Support Service-3Year(s)	1	354.00	354.00
	88032QRA-88134UHK-3	Basic Software License for Block(Include Device Management,SmartThin,SmartMulti-tenant,SmartMigration,SmartErase,SmartMotion,Cloud Service)-Hi-Care Application Software Upgrade Support Service-3Year(s)	1	738.00	738.00
Total of Service (3 years)					15,992.05
Total Price					141,391.33
Notes:Hi-Care Premier On-Site Service include: 7*24 Technical Assistance Center Access. Access to all new software updates and Online Support. 24*7*4 Hours Onsite Hardware Replacement.					